

Bergoz Instrumentation
 Espace Allondon Ouest
 01630 Saint Genis Pouilly, France
 Tel.: +33-450.426.642
 Fax: +33-450.426.643



Instrumentation


TECH NOTE IPCT-07/02
Integrated Parametric (DC)
Current Transformer

Rev. 1.0

IPCT-100mA typical response time is measured.

Maximum response time:
 Primary pulse to 50% output pulse amplitude: <130us
 Primary pulse to 90% output pulse amplitude: <250us

IPCT-100mA
Response time

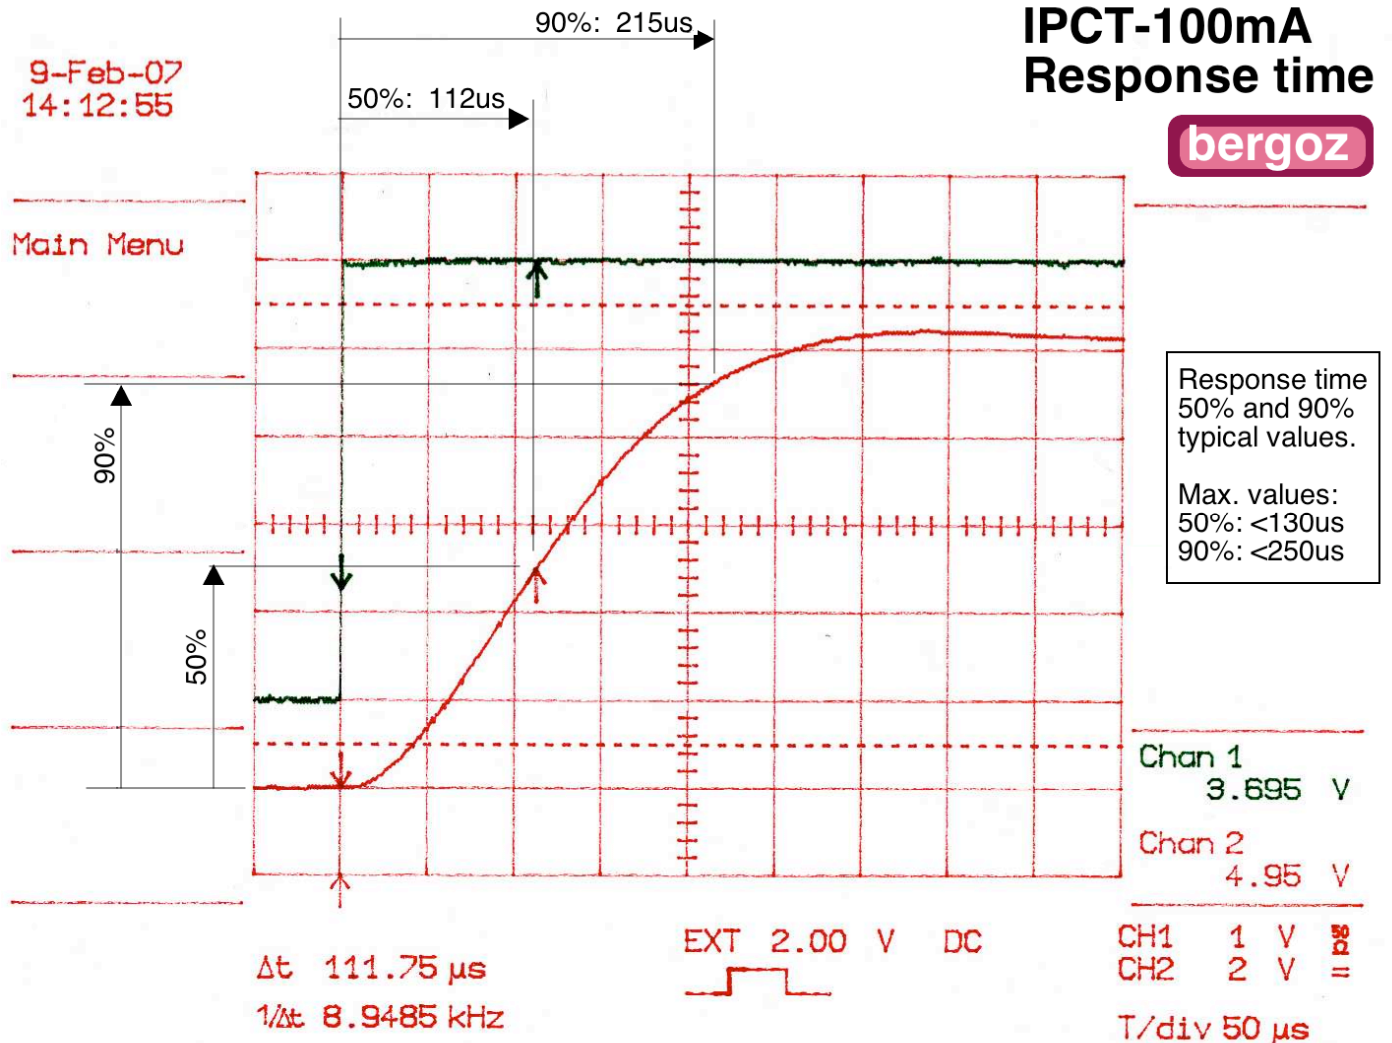

Data taken by Rémi Lubès, Tech Note authored by Julien Bergoz, Feb. 9, 2007