

Operation Manual for
Spectramag-6 Six-Channel Spectrum Analyser for Magnetic
Field, Vibration and LF Acoustics
SOFTWARE VERSION 6.203



Bartington®
Instruments

Table of Contents

List of Figures	6
1. About this Manual	7
1.1. Symbols Glossary	7
1.2. Key to Notation Used In This Manual	7
2. Safe Use	8
3. Important Points to Note Before Using the Spectramag-6	8
3.1. Compatible Sensors	8
3.2. Install the Software Before Connecting the USB Cable	8
3.3. PC Power Saving Features	8
3.4. Accidental Disconnection of the USB Cable	8
3.5. PC Power Drain	9
3.6. Saving Documents	9
3.7. Data Sampling – Aliasing	9
3.8. Compatibility	9
4. Introduction to Spectramag-6	9
4.1. Input Channels	10
4.1.1. Magnetometer Inputs	11
4.1.2. Accelerometer/Microphone Inputs	11
4.2. Sensor Ranges	11
4.2.1. Magnetometer Inputs	11
4.2.2. Accelerometer/Microphone Inputs	11
4.3. Coupling	12
4.3.1. Magnetometer Inputs	12
4.3.2. Accelerometer/Microphone Inputs	12
5. Hardware	12
5.1. Power Status and Charging	13
5.2. Controls and Connectors	14

5.3. Charging the Battery	14
6. Software	14
7. Connecting Spectramag-6 to the Computer	15
7.1. Connecting Subsequently	15
7.2. Disconnecting	16
7.3. Driver Reinstallation	16
8. Starting the Software	17
8.1. Scan Configuration Sub-Menu	18
8.1.1. Input Mode	19
8.1.2. Input Coupling	19
8.1.3. Display Type	20
8.1.4. Display Mode	20
8.1.5. Digital Filtering (Pre-Processing option)	21
8.1.6. Observing DC Trends	23
8.1.7. Acquiring AC signals	23
8.1.8. Setting Acquisition Modes	23
8.2. Specification Sub-Menu	26
8.2.1 Time Domain Specification	26
8.2.2 Frequency Domain Specification	27
8.3. Instrument Setup Sub-Menu	28
8.4. General Sub-Menu	30
8.5. Sensor Sub-Menu	31
8.6. FFT Sub-Menu	32
8.6.1 FFT Windows	32
8.6.2. Overlap Processing	33
8.6.3. Spectrum Selection	34
9. Acquiring Data	35

9.1. Quick Summary of Data Acquisition Using DC or AC Coupling	36
9.1.1. DC Coupling	36
9.1.2. AC Coupling	36
9.1.3. Process of Data Acquisition	37
10. Viewing Data and Annotating Displays	41
10.1. Zoom Control	41
10.2. Plot Settings	42
10.3. Plot Options	42
10.3.1. Data Sets	43
10.3.2. Show/Hide	43
10.3.3. Graph Title	43
10.3.4. Axis Titles	43
10.3.5. Axis	43
10.3.6. Axis Tick	44
10.3.7. Grid Lines	44
10.3.8. Key	44
10.3.9. Cursors	44
10.4. Show Cursor	44
11. Saving and Closing Files	45
12. Exporting Results	45
13. Data Recall and Processing	46
13.1. Digital Filtering	47
13.2. Averaging FFT Spectrum	49
13.3. Only Display Final Data Set	49
14. Operating Practice	50
15. Interpretation of Results	50
16. Troubleshooting	51

17. Maintenance	51
17.1 Changing the Battery	52
17.2. Shipping the Battery in this Equipment	53
Appendix A	54
A.1. Spectramag-6 Frequently Asked Questions (FAQ)	54
A.1.1. Sampling	54
A.1.2. Coupling	56
A.1.3. Windowing	57
A.1.4. Data Acquisition	57
A.2: Spectramag-6 Data Aquisition Choices Flowchart	59
A.3. Spectramag-6 Do's and Don'ts	60
Appendix B	62
B.1. Spectral Analysis using Fourier Transforms	62
B.1.1. Introduction	62
B.1.2. Fourier Series and Transforms	62
B.1.3. Processing digital signals	62
B.1.4. FFT windows	63
B.2.Sampling and Logging Time Estimates	65
Notes	66

List of Figures

Figure 1: The Spectramag-6 system connected to a magnetometer and an accelerometer	10
Figure 2: Spectramag-6 external connections	12
Figure 3: Spectramag-6 front panel	13
Figure 4: The Settings Menu showing the six sub-menus	18
Figure 5: The Scan Configuration sub-menu of the Spectramag-6 software	19
Figure 6: An acquired signal in a noisy environment	22
Figure 7: Setting the Pass/Fail limits in the Spectramag-6 software	27
Figure 8: Test failure when the measured signal exceeds the set limits	28
Figure 9: The Instrument Setup sub-menu	29
Figure 10: The General sub-menu	30
Figure 11: The Sensor sub-menu	31
Figure 12: FFT settings for the Spectramag-6 software	33
Figure 13: Time and Frequency Domain plots from Spectramag-6	37
Figure 14: Process of data acquisition	38-41
Figure 15: Changing the display modes	42
Figure 16: Spectramag-6 Plot settings	43
Figure 17: Changing plot parameters	44
Figure 18: Using cursors in Spectramag-6	46
Figure 19: The post processing feature in the Spectramag-6 toolbar	48
Figure 20: The Spectramag-6 post processing window	48
Figure 21: (a) Data acquired in a noisy environment and (b) the data after low-pass filtering	49
Figure 22: Signals from two logged data files	50
Figure 23: Opening multiple windows in the Spectramag-6 software	51
Figure 24a: Internal battery location	53
Figure 24b: Battery clamped to top of assembly, with rubber foot attached	53
Figure A.1: A diagram illustrating how the resolution of a frequency plot can be chosen	56
Figure A.2: Flowchart showing suitable choices for data acquisition using the Spectramag-6 software	60
Figure B.1: Aliasing due to undersampling a signal	64

1. About this Manual

This document describes the installation, operation and maintenance of the Spectramag-6 system from Bartington Instruments. It should be read in conjunction with the [product brochure](#) (DS2519) which can be found on the product page of the Bartington Instruments at: www.bartington.com.

Spectramag-6 software can be downloaded from the [software page](#) of the website.

A block diagram showing the Spectramag-6 system can be found on the [drawing page](#).

1.1. Symbols Glossary

The following symbols used within this manual call your attention to specific types of information:



WARNING: Indicates a situation in which serious bodily injury or death could result if the warning is ignored.



Caution: Indicates a situation in which bodily injury or damage to your instrument, or both, could result if the caution is ignored.



This symbol identifies items that must be disposed of safely to prevent unnecessary damage to the environment.

Note: A note provides useful supporting information and sometimes suggests how to make better use of your purchase.

1.2. Key to Notation Used In This Manual

Menu items, tabs, check-boxes and other selectable ('clickable') items displayed in the software are shown in this manual in **bold letters**, e.g. "click on the **OK** button".

A sequence of actions is shown using arrows. Hence, for example:

- **Edit → Copy** means "select **Edit**, then select **Copy**".
- **Control Panel → System and Security → Device Manager** means "click on Control Panel, then System and Security, then Device Manager".

Note: The user's familiarity with different versions of the Windows operating system is assumed. Hence, for example, an instruction might be to 'open **Control Panel**' rather than a detailed description of the route to follow to get to Control Panel, as these steps will not necessarily be the same from one version of Windows to the next.

2. Safe Use



WARNING: These products are not qualified for use in explosive atmospheres or life support systems. Consult Bartington Instruments for advice.

3. Important Points to Note Before Using the Spectramag-6

3.1. Compatible Sensors

The Spectramag-6 unit is for use only with the devices listed below:

- Sensors from Bartington Instruments Ltd listed in the compatibility table at: www.bartington.com/product-compatibility.html.
- Accelerometers with ICP interface from PCB Piezotronics Inc., e.g. 393A03 (1V/g) or 393B31 (10V/g).
- Microphone 40AE with preamplifier 26CA from G.R.A.S. Sound and Vibration.



Caution: The connection of any other device may cause serious damage and will invalidate the equipment warranty.

3.2. Install the Software Before Connecting the USB Cable



Caution: The Spectramag-6 software must be installed on your PC before attempting to connect the hardware using the USB cable. Connection of the hardware prior to installing the software may cause the system to malfunction.

3.3. PC Power Saving Features

Note: PC power saving features (e.g. hibernation, sleep mode, screensavers, etc.) have been known to cause problems when using the Spectramag-6 system, and to prevent the system from logging data correctly. These features should be disabled whilst the Spectramag-6 system is being used. Consult your PC's documentation for instructions on how to do this.

3.4. Accidental Disconnection of the USB Cable

Note: Disconnection of the USB cable whilst the Spectramag-6 system is operating may cause the system to malfunction. Should this occur, stop the PC program, reconnect the USB cable, wait 15 seconds and then re-start the program.

3.5. PC Power Drain

Note: Under normal operation, power is supplied to the Spectramag-6 unit from its internal batteries. However, if the Spectramag-6 unit is switched off but connected to a PC with the PC switched ON, then power will be drawn from the computer (approx. 240mA). For a laptop PC this may affect battery life. Avoid leaving an un-powered Spectramag-6 unit connected to a laptop PC that is switched on.

3.6. Saving Documents

Note: The My Documents folder should not be used as a location for saving data when automatically logging multiple files using the Multiple Acquisition mode. Files can only be saved in the My Documents folder manually, for example when a single run is made using the Single Acquisition mode.

3.7. Data Sampling – Aliasing

Note: Always use a sampling frequency that is adequately high to avoid aliasing. For example, a 60Hz signal caused by mains electricity can contain harmonics of significant magnitude up to 240Hz. See [Digital Filtering](#) for steps to minimise or eliminate aliasing.

3.8. Compatibility

Note: Version 6 software is compatible with earlier versions. Files created in the earlier versions can be opened and post-processed. See also [Software](#).

4. Introduction to Spectramag-6

The Spectramag-6 system, comprising the Spectramag-6 hardware and software, provides a PC-based, fast, six-channel, 24-bit data acquisition system with data logger and spectrum analyser for Bartington Instruments fluxgate sensors, and for industry standard ICP accelerometers and microphones. The Spectramag-6 system performs simultaneous data acquisition in all six channels and produces both time domain and frequency domain plots showing either slow or fast trends for magnetic, vibration and sound data in three axes.

Time-varying information is converted into a frequency spectrum using Fast Fourier Transforms, referred to as FFT in the text. When the Spectramag-6 is used as a data logger, time-stamped data can be logged (for extended periods), and then retrieved and post-processed in both time and frequency domain. The system is software controlled with connection to the user's PC via a USB interface. Prior to data acquisition, the system is configured using the Spectramag-6 software. A typical arrangement is shown in **Figure 1**.

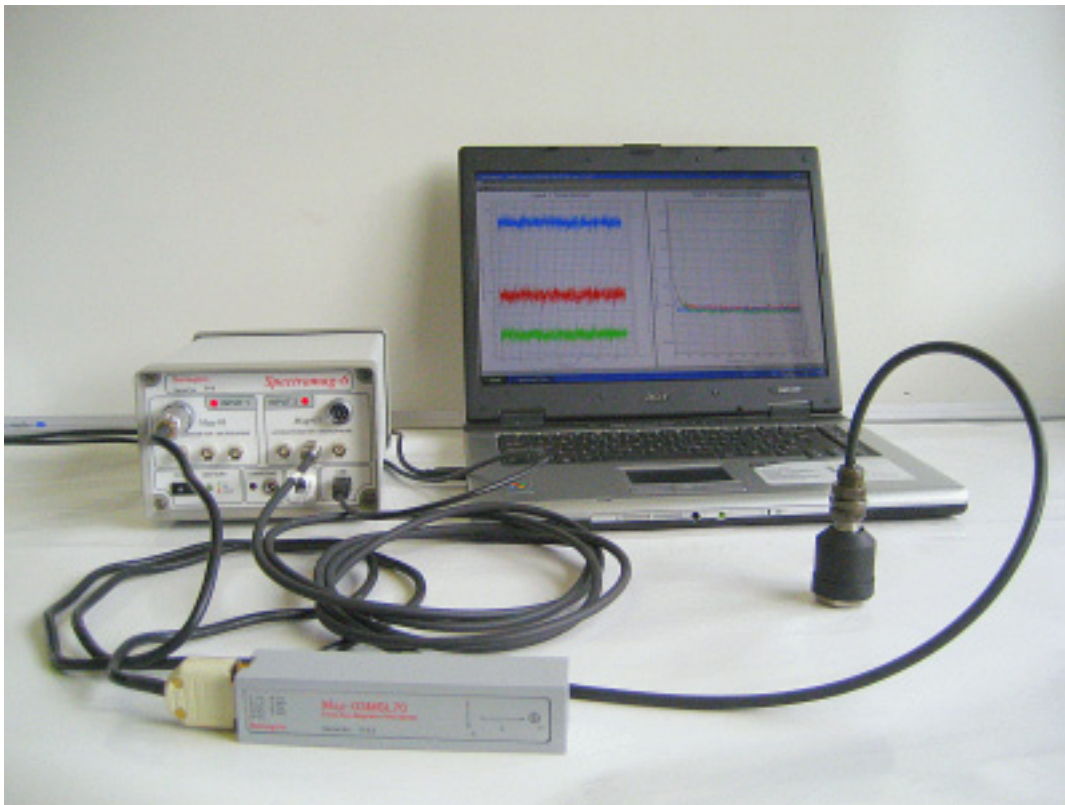


Figure 1: The Spectramag-6 system connected to a magnetometer and an accelerometer.

The Spectramag-6 software records time and frequency domain data over a wide frequency range (see the product brochure for details). Data logging with time-stamping is also provided, hence the system functions as a high-resolution data logger for magnetic, vibration and sound measurements. The Spectramag-6 software is compatible with 32 and 64 bit versions of Windows 7, Windows 8 and Windows 8.1. It is also compatible with Windows 98, Windows NT, Windows 2000, and Windows XP 32 bit.

4.1. Input Channels

The six input channels are divided into two groups of three (Input 1 and Input 2) and are marked on the front panel of the hardware as follows:

Group	Channels	Sensor Type
Input 1	X, Y, Z	Select all 3 channels as magnetic or acceleration or pressure
Input 2	X, Y, Z	Select all 3 channels as magnetic or acceleration or pressure

A user can activate either or both groups of inputs for data acquisition and display.

Note: sensor types on the three channels of an input group cannot be mixed.

Valid combinations are:

- Two compatible Bartington sensors (on Input 1 and Input 2).

or

- One compatible Bartington sensor, and up to 3 accelerometers or up to 3 pressure sensors.

or

- Up to 3 accelerometer or 3 pressure sensors on one input group and up to 3 accelerometer or 3 pressure sensors on the other input group.

4.1.1. Magnetometer Inputs

When a compatible Bartington Instruments triaxial magnetometer is connected to the system, the X, Y, Z channels correspond to the X, Y, Z axes of the magnetometer. Hence, up to two compatible magnetometers can be connected to the Spectramag-6 data acquisition system via the two circular 10-way connectors at the front of the unit.

4.1.2. Accelerometer/Microphone Inputs

When connecting an accelerometer or a microphone to the system, the two input groups (Input 1 and Input 2) can be independently selected for vibration/acceleration or sound/pressure measurements. The Accelerometer/Microphone inputs are six separate BNC connectors on the front panel. These inputs use ICP interfaces that provide a 4mA constant current source, and are compatible with ICP accelerometers and ICP microphone/preamplifier combinations.

4.2. Sensor Ranges

4.2.1. Magnetometer Inputs

The Spectramag-6 system is designed to accommodate the full scale ranges of compatible Bartington magnetometers.

4.2.2. Accelerometer/Microphone Inputs

The Spectramag-6 has preset accelerometer input scaling values, or a custom value can be set by the user to match the scaling of the sensor being used.

The microphone input has a custom scaling which can be set by the user, to match the mV/Pascal scaling of the sensor in use.

4.3. Coupling

4.3.1. Magnetometer Inputs

Magnetometers can be DC or AC coupled to the Spectramag-6 unit via a high-pass filter.

4.3.2. Accelerometer/Microphone Inputs

The ICP interface connectors supply a constant DC current to the sensors. Input coupling is AC.

5. Hardware

A Spectramag-6 system in typical use (say, in an MRI survey) comprises a Spectramag-6 unit, a compatible three-axis magnetometer, a connecting cable, a tripod for the magnetometer, a USB cable, universal mains adaptor, and up to three accelerometers with optional microphone and preamplifier with associated cables. All items can be conveniently accommodated in an optional rugged carrying case offered with the Spectramag-6 system. The user's laptop computer (with a USB interface and installed software) completes the system. Connections to the Spectramag-6 unit for a typical application are shown in **Figure 2**.

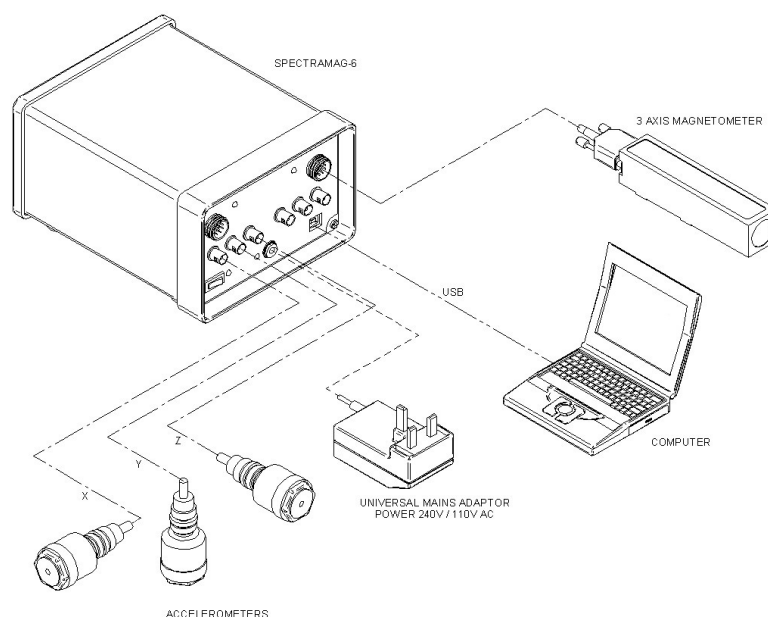


Figure 2: Spectramag-6 external connections.

The Spectramag-6 unit contains power supplies, amplifiers, filters, six simultaneously triggered 24-bit A/D converters and a USB interface. To allow field work with a laptop computer, the unit contains an internal Lithium Ion battery which is recharged via the universal mains adaptor supplied. In order to optimise the battery life of any laptop to which the unit may be connected, power to the USB interface is provided by the internal battery of the Spectramag-6 unit. In order to extend battery operation, magnetometer power is applied only to the sensor group or groups selected.

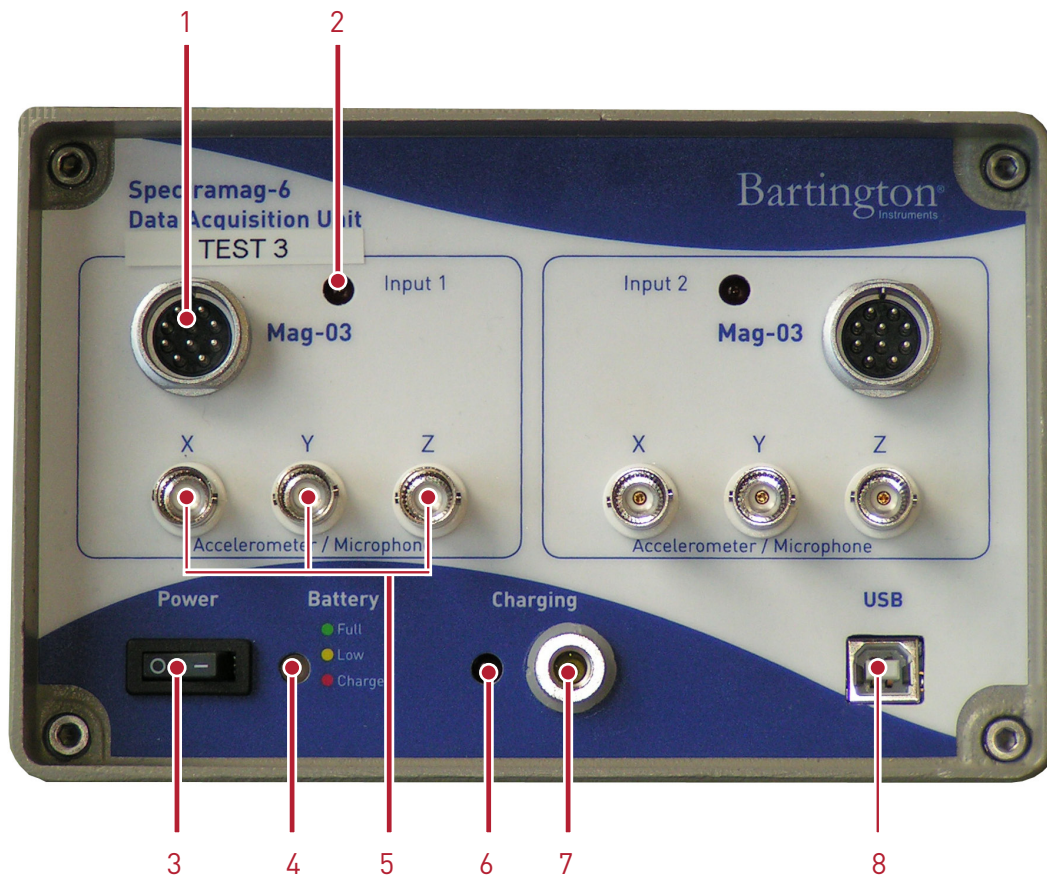


Figure 3: Spectramag-6 front panel.

Key to Figure 3

1. Hirose magnetometer connector for input 1 (duplicated for input 2)
2. Input 1 indicator light (duplicated for input 2)
3. ON/OFF switch
4. Battery status indicator light
5. BNC connectors for accelerometers or microphones for input 1 (duplicated for input 2)
6. Charging indicator light
7. Charging socket for mains adaptor
8. USB port

5.1. Power Status and Charging

A power-on switch [3] is situated at the bottom left hand side of the front panel with a battery status indicator [4] (**Figure 3**). When the unit is switched ON, the battery status indicator shows green if the battery is fully charged; amber if the charge is low; and red if it is very low.

Note: When the indicator shows red, the unit should not be used but should be recharged until the indicator shows green.

The unit may be operated while recharging. The charging socket for the mains adaptor [7] has an indicator [6] that is lit when the battery is being charged.

Note: For prolonged on-site measurements, additional power sources should always be provided.

5.2. Controls and Connectors

All the controls and connectors of the unit are on the front panel as shown in **Figure 3**. The input connectors for the sensors are arranged in two groups, each group having one Hirose magnetometer connector [1] and three BNC connectors [5] for accelerometers or microphones.

A compatible three-axis magnetometer or up to three accelerometers or microphones may be connected to each input group. The unit provides the power for the compatible magnetometers and a constant current ICP interface for the accelerometer and microphone inputs as required. A block diagram of the unit is shown on the Spectramag-6 product page.

The BNC connectors (**Figure 3**) are labelled X, Y and Z to correspond to the allocated data channel. A front panel red indicator [2] is lit when power is applied to each group. A USB connector is situated at the bottom right hand side of the front panel for connecting to the PC [8].

Note: The unit must not be connected to a PC until the Spectramag-6 software has been installed.

5.3. Charging the Battery

The battery should be fully charged before use. Connect the universal mains adaptor supplied to the Charging socket and apply power. The Charging indicator should be illuminated and should change from red to amber to green as the charging progresses.

Note: Adequate charging should be done before use, i.e. the charging indicator should at least show the amber colour. Otherwise the performance of the Spectramag-6 system cannot be guaranteed.

A full charge takes about 10 hours and the charging will terminate automatically at the end of this time, although the indicator will still be illuminated.

See also [Maintenance](#).

6. Software

The Spectramag-6 system is supplied complete with dedicated data acquisition software. Consult Bartington Instruments for the minimum hardware requirements and installation instructions.

A summary of how to use the Spectramag-6 software is given as a flowchart in **Figure A.2** - see Appendix. Available versions of the Spectramag-6 software can be downloaded from www.bartington.com/software.html.

Note: A small change is made to the Spectramag-6 firmware when operated with version 6.203 of the software or later. After the Spectramag-6 has been run with this version, it will be incompatible with earlier versions of the software. However, the change can be reversed with a **system reset**. This is performed by removing the mains and USB cables from the unit, and switching the power off. This should be done before connecting the Spectramag-6 to a different computer and after any re-installation of the software.

7. Connecting Spectramag-6 to the Computer

Note: The Spectramag-6 unit should only be connected to a computer running Windows.

After installing the software, connect the required sensors to the Spectramag-6 unit and switch the unit ON using the front panel switch. Connect the Spectramag-6 unit to the PC using the USB cable supplied. Windows should detect the instrument automatically. The user will be prompted to load device drivers the first time the instrument is connected. The drivers are located on the CD but are also installed in the program folder.

1. To use the copy on the CD, simply select the drive in the menu and click **OK**.
2. To use the installed drivers, click the option allowing the location of the drivers to be specified and browse to the Spectramag-6 installation folder.

Note: The default option is C:\Program Files\Bartington Instruments\Spectramag-6, but the program may also be installed at any other location.

3. Click on the CIL.inf file and click **Open**.

Some operating systems may request the driver a second time, hence steps (2)–(3) should be repeated. A message may now appear indicating that a new USB device has been found and that this is a Bartington Input Device. If shown, these messages should disappear automatically after a few seconds. The instrument is now ready for use.

7.1. Connecting Subsequently

After the procedure above has been performed for the first time, the necessary drivers will reside in the PC for future use. If the instrument is re-connected subsequently, it will be detected automatically and the drivers will be loaded without further intervention. Firstly, connect the sensors required, and then switch ON the power to the Spectramag-6 unit. Finally, connect the Spectramag-6 unit to the computer with the USB cable. Allow 10-15 seconds for the unit to start communications and then start the Spectramag-6 program. See also [Operating Practice](#).

7.2. Disconnecting

Carry out the reverse of the connection process. With the Spectramag-6 program closed, disconnect the USB cable from the PC before switching off the Spectramag-6 unit. (Disconnecting the USB cable when the unit is still 'live' will minimise current drain from the computer battery.) See also [Operating Practice](#).

7.3. Driver Reinstallation

It may be necessary to reinstall the driver software: for example when the USB cable is accidentally disconnected, but the Spectramag-6 unit cannot now be detected despite reconnecting the USB, waiting 15 seconds, and running the Spectramag-6 software.

Follow these steps to re-install the device driver:

1. Open **Control Panel** on your PC.
2. Go to **System → Hardware → Device Manager**.
3. Double-click on the Universal Serial Controller.

Note: If a (Bartington) USB device is seen with a yellow sign, the driver is not properly installed and should be reinstalled.

4. Double-click the USB device (with the yellow sign) and click **Update Driver**. A Hardware Update Wizard window opens. Select '**Yes, this time only**', then click **Next**.
5. Select '**Install from a list of specified location**', then click **Next**.
6. Select '**Don't search I'll choose a driver to install**', then click **Next**.
7. Click on **Browse** and either go to the location where Spectramag-6 is installed on the PC, or go to the folder on the Spectramag-6 CD.
8. Click on a file named CIL.inf and click **Open**.
9. Click **Next** and click **Continue Anyway** in the following windows.
10. Now open the Spectramag-6 software.

If there is still no connection to the Spectramag-6 unit, close the Spectramag-6 program, switch OFF the unit and disconnect the USB cable. Switch the unit ON again and connect the USB cable; wait 15 seconds and start the Spectramag-6 program. Windows should detect the Spectramag-6 unit as a Bartington Instrument device. If this is not the case, repeat processes 1 to 9 [because some operating systems want this process to be done twice] and restart the PC.

The above processes should properly install the device driver enabling connection to the Spectramag-6 unit.

8. Starting the Software

When the Spectramag-6 unit has been connected and powered up, start the software by either double clicking on the Spectramag-6 desktop icon or by selecting Spectramag-6 from the Bartington Instruments folder in the Windows Start menu. On start-up, the software will automatically detect a connected instrument and list it as BRT01. If there are several items in the list then select **BRT01**, otherwise just click **OK** to initialise communications. If the instrument is not detected on starting the software, select **Tools → Detect Instruments** from the toolbar menu. Alternatively, re-install the driver (see previous section). When the device has been found, certain parameters such as the sampling rate, the number of samples etc. need to be set up before running a scan.

Data is sampled, processed and displayed under software control using parameters set by the user. These parameters are set from menus and saved as default parameters for use in subsequent scans. The user can set the inputs to be used, the sampling rate, gain settings, input coupling, and display options. To set up the software, click the  icon on the toolbar or select **Scan → Configure**. This brings up the **Settings** menu. As shown in **Figure 4**, this has five sub-menus that must be used for defining the operation of the software, and an optional sixth (**Specification**) sub-menu. The settings in the Specification sub-menu are only required to set Pass/Fail limits for any measurement (see [Specification Sub-Menu](#) for further details).

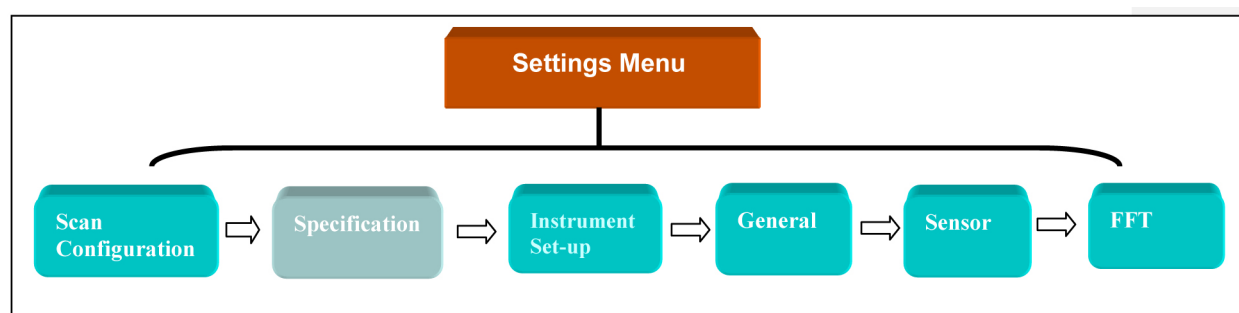


Figure 4: The Settings Menu showing the six sub-menus

The use of each sub-menu is shown in **Table 1**.

Table 1: The use of each sub-menu.

Scan Configuration	Select input device, coupling, sampling frequency, number of samples, filtering, display mode.
Specification	Set Pass/fail limits for detecting when a signal reaches a set limit.
Instrument Set-up	Set the input gain of the system.
General	Specify a location to save their data to, and whether or not data should also be saved in ASCII format.
Sensor	Set sensor units and scaling.
FFT	Select frequency domain parameters such as FFT windows.

The options selected in the six sections of the **Settings** menu will be saved automatically on exit (as default values to use in a run) when the **OK** button is selected. When a run is completed, the settings used in the run are saved for use in the next run. If however the run is terminated (say, by stopping the program) then the settings for the most recent completed run will be loaded automatically whenever a new run is started. The user can also save these settings to a file by clicking the **Save Scan Template** button in **Figure 5**. To use an already saved template, click **Load Scan Template**. On selecting the **OK** button, the unit will automatically set the offset of all magnetometer inputs to zero. If the **Scan on Exit** box (found under the **General** sub-menu) has been selected, a scan will then be initiated automatically when the **OK** button is clicked. In the following sub-sections each of the sub-menus in **Figure 4** will be discussed.

8.1. Scan Configuration Sub-Menu

The Scan Configuration sub-menu is the default menu that appears after selecting **Scan → Configure** as shown in **Figure 5**. The top of the menu is divided into two sections, one for Input 1 and the other for Input 2. (Input 1 and 2 represent the two input groups of the Spectramag-6 system, as mentioned in [Input Channels](#).)

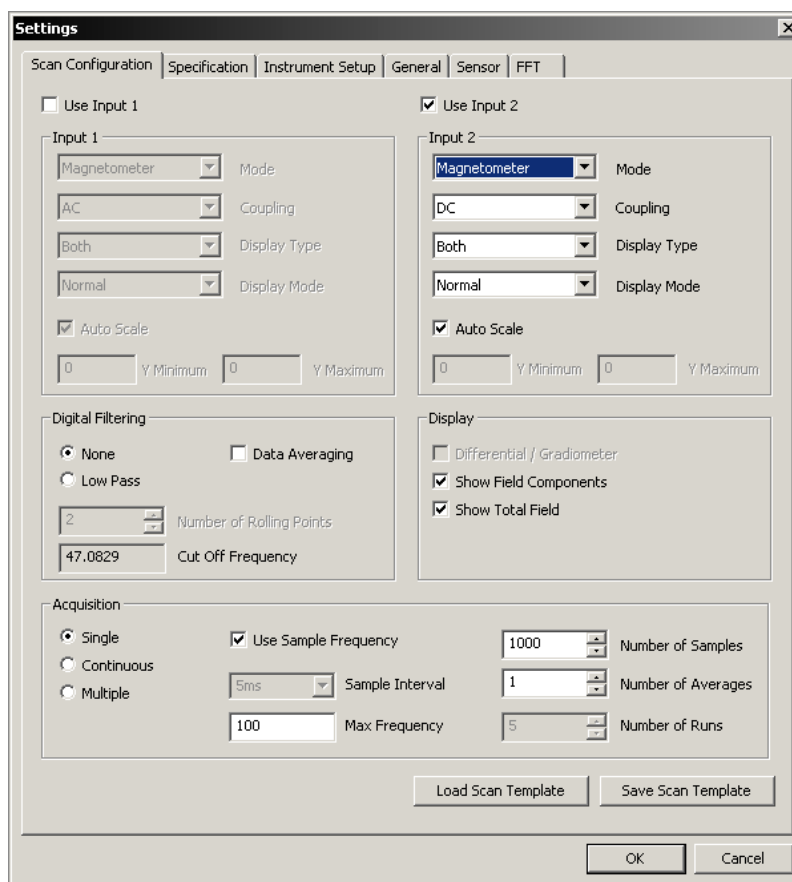


Figure 5: The Scan Configuration sub-menu of the Spectramag-6 software.

8.1.1. Input Mode

At the top of each section is a 'Use Input' box for selecting whether or not an input is to be used. Tick a box to select an input to be used and leave blank if an input is not required. If a box is selected then the **Mode**, **Coupling**, **Display Type** and **Display Mode** options become live.

For each input selected, the type of input device can be set as a **Magnetometer**, **Accelerometer** or **Microphone** via the **Mode** drop-down menu. Select the appropriate sensors to be connected to Input 1 and /or Input 2.

8.1.2. Input Coupling

Because magnetometers have a response containing both DC and AC components, when a magnetometer is selected, the coupling to the Spectramag-6 (hardware) inputs can be selected as either **DC** or **AC**. Hence DC coupling can be used to allow both AC and DC components, or AC coupling can be used to only allow AC components.

Accelerometers and microphones however only have AC response; hence, AC coupling is the only option that can be selected for these. The DC coupling option is greyed out once the **Accelerometer** or **Microphone** input is selected. The bandwidth of the accelerometers and microphone inputs is limited internally by a high-pass filter with a -3dB point fixed at 0.1Hz

regardless of the coupling selected. The selection of AC or DC coupling therefore only applies to the magnetometer inputs.

When using a magnetometer input, DC coupling should normally be selected as the default. However, if a gain of greater than one is required to view a small AC signal which may be superimposed on a large DC magnetic field, then the resulting DC level may cause the Spectramag-6's input amplifiers to saturate, due for example to the background fields. The AC response may then be used to remove the unwanted DC input component prior to amplification to allow investigation of the AC component only.

Note: The AC input coupling should be used with care as it gives the same appearance to the display as the Mean Zero or Offset to Zero display modes described below. The difference is that **Display Mode** (comprising the Normal, Mean Zero and Offset to Zero modes: see [Display Mode](#)) is used for analysing acquired data containing both AC and DC components, and allows the DC component to be added or removed from the dataset during analysis. AC coupling filters out DC components permanently during data acquisition, i.e. they are removed before recording and cannot be retrieved.

See [Acquiring Data](#), for more on AC and DC coupling.

8.1.3. Display Type

The **Display Type** menu allows **Time Domain**, **Frequency Domain** or **Both** to be selected for display. The display selection can be changed as required after completion of a scan using the **View** option of the display window.

8.1.4. Display Mode

The **Display Mode** for each input section allows **Normal**, **Mean Zero** or **Offset to Zero** to be selected. These apply only to the time domain data but the frequency domain plot will be affected by the inclusion or removal of quasi-DC components when **Mean Zero** or **Offset to Zero** modes are used. The **Display Mode** selection can also be changed as required after completion of a scan.

Normal Mode	In the Normal mode the time domain plots represent the real data (including both AC and DC components). As a post processing feature, one can switch between the Normal mode and the other display modes for comparisons.
Mean Zero Mode	In Mean Zero mode Spectramag-6 calculates the mean value of the X, Y and Z dataset (the sum of all points divided by the number of points) and subtracts this from the total value of the X, Y and Z dataset.

Offset to Zero Mode	The Offset to Zero mode calculates the mean value of the first 10 points of an input and subtracts this value from all of the individual data points. This causes each trace to start at or near the zero line and is useful for measuring/comparing relative changes (i.e. excursions) in the three components of the magnetic field, or for comparing inputs from different accelerometers/microphones over a period.
----------------------------	--

Display Scaling

The **Auto Scale** box, if ticked, will provide automatic scaling of the graphs to accommodate the data. If the box is not ticked, the maximum and minimum values for the Y-axis must be specified. Note that the values to be entered in the box will be multiplied by the scaling set (from the **Sensor** sub-menu, see **Figure 11**): hence to set a range, for example, from 0 to $0.08\mu\text{T}$ when ' μT ' is checked in the Sensor sub-menu, enter '0' and '0.08' as the Y Minimum and Y Maximum respectively. This allows scans to be run with the same scale for comparisons. The **Auto Scale** enable/disable feature only works on the time domain plots; i.e. the ranges of the frequency domain plots are set automatically by the program.

Additional Display Settings

If a magnetometer is selected for an input then the **Show Total Field** box can be ticked. This will cause the total field to be calculated from the square root of the sum of the squares of the three field values and displayed as a fourth component. This can be used in combination with the **Show Components** box to display the individual components and/or the total field. If magnetometers are used for both inputs then ticking the **Differential / Gradiometer** box will cause the graph for Input 1 to remain unchanged, but in place of the plot for Input 2, an Input2 – Input 1 graph will be displayed showing the difference between the magnetometer inputs.

Note: The number of data-points should be limited to 100,000 points when using both the Show Total field and the Differential/Gradiometer option.

8.1.5. Digital Filtering (Pre-Processing option)

Two radio buttons and a check box are grouped under '**Digital filtering**' in the **Scan Configuration** sub-menu.

The two radio buttons available are:

1. **None.** If selected, no digital filtering is applied to the acquired data prior to it being displayed in time and/or frequency.
2. **Low Pass.** This button causes a variable Moving Average low-pass filter to be applied to the data (**Figure 6**). The number of points to use for averaging is set using an up-down arrow labelled '**Number of Rolling Points**' (NRP). The cut-off frequency of the filter is given in the text box labelled 'Cut Off Frequency' and depends on the sampling frequency and the NRP.

The low-pass filter can be used generally for reducing the appearance of power line signals (e.g. 50Hz or 60Hz) when for example only slow magnetic trends are of interest. This filter is applied to the incoming data in real-time, therefore information above the cut-off frequency will be permanently lost.

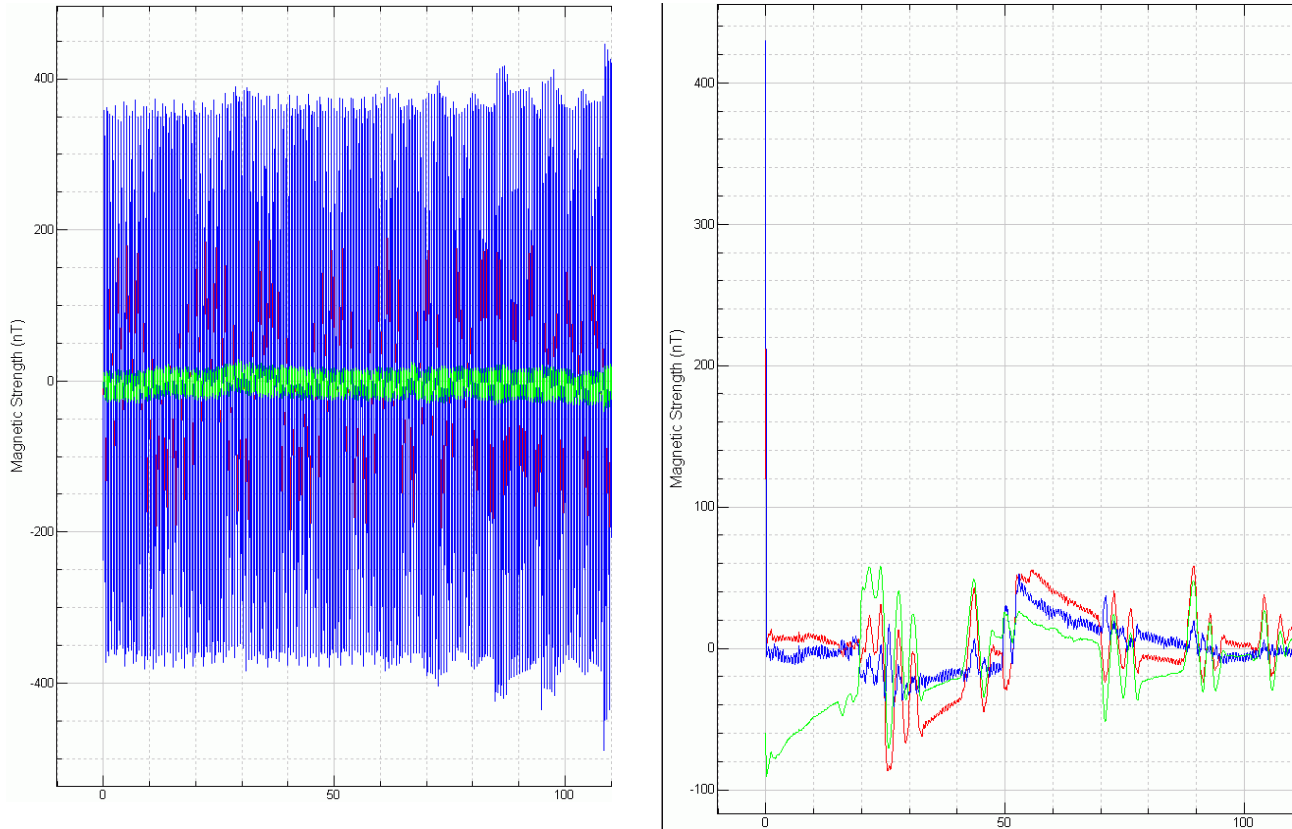


Figure 6: An acquired signal in a noisy environment. (6a) With the low-pass filter OFF, the noise obscures the desired signals. (6b) The effect of applying a low-pass ($f_{\text{cut-off}} = 2\text{Hz}$).


Note: The low-pass filter is **not** primarily an anti-aliasing filter, given that it is a software filter positioned after (not before) the A/D converter. As such, signals must be sampled fast enough (at least at two times the highest frequency component in the input signal, according to the Nyquist criterion) in order to have them resolved in frequency. Once the correct sampling frequency is used (i.e. no aliasing), the following low-pass filter is used to eliminate unwanted signals from the displayed frequency spectrum. **Where the user suspects that aliasing will be a problem, the Data Averaging feature should be used to reduce this effect.**

Data Averaging

When **Data Averaging** is selected, the system will use multi-rate sampling to minimise aliasing effects. When the **Data Averaging** check box is ticked, and data sample interval is 1ms or longer, the system is forced to acquire data at a higher sampling frequency. Data is then averaged and final data is stored at the rate selected by the user. This multi-rate sampling is not apparent to the user and no allowance needs to be made for it. Its purpose is simply to minimise the aliasing effects that can occur where simple sampling is used, and frequencies above the Nyquist

frequency are present in the signal being measured. This often occurs in the investigation of low frequency signals, with 50 or 60Hz present.

If a sample interval of longer than 1ms is selected, and **Data Averaging** is not checked, then the system will issue a warning that aliasing is a danger (right).

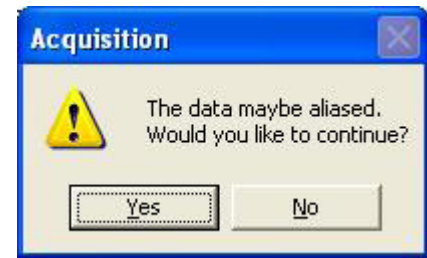

If the user responds 'Yes' then the scan will commence, but multi-rate sampling will not be used; data is acquired at the sample rate specified by the user, and aliasing may occur if frequencies above the Nyquist frequency are present.

Data Averaging can be used with or without the other digital filter settings.

8.1.6. Observing DC Trends

The following steps should be taken for setting the filter values. Let us assume for example that a slow signal of frequency between 0.1–5Hz is to be acquired:

- (a) Set the sampling frequency to a minimum of 10Hz according to the Nyquist criterion (i.e. set Max Frequency to 5 in the Spectramag-6 program).
- (b) Adjust NRP using the up-down arrow to set the cut-off frequency **below the power line frequencies** (50 or 60Hz). The cut-off frequency decreases as the NRP is increased.

To reduce the effect of power line signals substantially in the time domain plots (in order to observe DC trends, for example during site surveys), the cut-off frequency should be set, say, between 1.5–10Hz. The effect of applying the low-pass filter is shown in **Figure 6**.

8.1.7. Acquiring AC signals

The key requirement in this case is to set the sampling frequency to a minimum of twice the maximum frequency in the signal according to the Nyquist criterion. The Nyquist criterion **must** be met at all times to avoid aliasing. Assuming that a signal of 200Hz needs to be acquired:

- (a) Set the sampling frequency to a minimum of 400Hz according to the Nyquist criterion (i.e. set Max Frequency to 200 in the Spectramag-6 program).
- (b) Adjust the NRP using the up-down arrow to set the cut-off frequency **above the desired signal frequency, say to 300Hz**, or turn the low-pass filter OFF.

8.1.8. Setting Acquisition Modes

Data can be acquired using three different acquisition modes:

1. Single.
2. Continuous.

3. Multiple.

Table 2 shows the parameters that need to be set for each data acquisition mode.

Table 2: Parameters that need to be set for each data acquisition mode

Acquisition mode	Max Frequency	No of Samples	No of Averages	No of Runs
Single	✓	✓	✓	--
Continuous	✓	--	Set to 1	--
Multiple	✓†	✓	--	✓
✓ = Needs to be set -- = Not used				

Single Mode	The Single data acquisition mode, as the name implies, is used to execute a single run of the program to acquire data once. As shown in Table 2 the user needs to set the sampling frequency (f_{samp}) by setting Max Frequency (which is $f_{\text{samp}}/2$), the number of samples and the number of averages. The acquired data can be manually saved by selecting File → Export → Data and selecting the location and the name of the data file to be created.
Continuous Mode	The Continuous mode provides a data logging facility for acquiring very low frequency signals in the order of 0.1Hz or less (such as seismic waveforms etc). This function is activated by checking the Continuous Acquisition box. During continuous data acquisition the maximum sampling frequency is 0.2Hz, corresponding to a sampling period of 5 seconds. Data can be saved at the end of a run (or by stopping the program using the  icon on the toolbar) by selecting File → Export → Data and selecting the location and the name of the data file to be created.
Multiple Mode	The Multiple mode feature allows continuous data logging to be accomplished by the Spectramag-6 software. The user has to set the sampling frequency f_{samp} (by setting Max Frequency which is $f_{\text{samp}}/2$); the number of samples (N); and the number of runs (R). A minimum of 2 runs is required when using the Multiple mode. In this mode, data is continuously logged to the hard disk as multiple (R) data files with each file containing N data points. The data in each file is also time-stamped to aid future analysis. It has been estimated that the dead-time between consecutive files is approximately 2 seconds. This test was done using an AMD Athlon, 64 X2 Dual Core, 2.01GHz, 1GB RAM computer.

Note: In **Multiple** mode, data is automatically logged to the hard disk as .sm6 files and as ASCII files if this option is selected under the **General** sub-menu. The location of the data files is specified by clicking the **General** sub-menu as shown in **Figure 10**.

Sampling Frequency

Ticking the **Use Sample Frequency** box lets you set the sampling frequency for each scan as a frequency value ' f '. Values can be entered into the Max Frequency box. This is half the sampling frequency, i.e. $\text{Max Frequency} = f_{\text{samp}}/2$. The Max Frequency also represents the Nyquist frequency, hence the range of the frequency domain plots is from zero up to Max Frequency.

Leaving the **Use Sample Frequency** box unchecked means you must specify the sampling period ($T = 1/f$). If the **Use Sample Frequency** box is not ticked, the **Sample Interval** box is then activated from where sampling period ($T = 1/f$) values can be chosen ranging from 100µS to 10S.

Number of Samples

The Spectramag-6 system allows a maximum of 700,000 data points to be acquired during each scan, both for normal scan and continuous data acquisition. The number of samples to be used for a scan is set by entering a value in the **Number of Samples** input box.

Number of Averages

The **Number of Averages** dialogue box sets the number of scans to be averaged for the frequency domain display.

Note: The time domain display is not averaged and the display shows the latest scan.

Selecting a number of averages (say, N greater than one) will increase the scan time by N times but the averaging reduces the noise in the spectrum plot by integration.

Number of Runs

This is used only when **Multiple** data acquisition mode is selected to set how many completed acquisition runs the program should make. Given that a file is saved at the end of each run, this feature also sets the number of complete data files that should be produced/logged to the hard disk.

Save/ Load Scan Template

Clicking the **Save Scan Template** button allows a user to save (as a .smt file) all the settings made by the user (in all the **Settings** sub-menus). This could be a set of favourite settings for a particular test. To load a saved template, click the **Load Scan Template** button, select the template file to be loaded and click **OK** to load the template.

Note: The **OK** button MUST be clicked to load a template properly.

8.2. Specification Sub-Menu

The **Specification** sub-menu lets the user set values (for time or frequency domain or both) that will cause a test to fail when exceeded. The user-defined pass/fail limits apply to all input groups. The values set might correspond to acceptable magnetic field, vibration or sound levels during a test, or in the case of an MRI site survey, might correspond to an equipment manufacturer's specification. A pass/fail limit is set from the **Scan** → **Configure** → **Specification** tabs as shown in **Figure 7**.

Note: To use the Pass/Fail feature, set the Display Mode ([Display Mode](#)) to **Offset to Zero** to display only the true amplitude of the signal detected, i.e. without showing DC offsets.

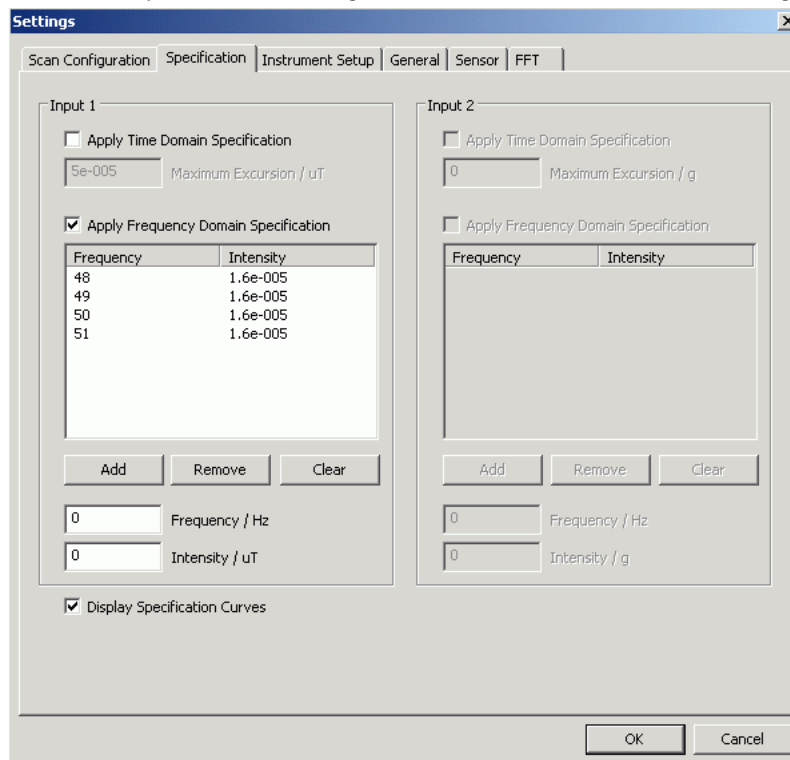


Figure 7: Setting the Pass/Fail limits in the Spectramag-6 software.

A test pass or fail is indicated at the bottom of the output display. From Version 6 of the software, an audible beep is also used to indicate a fail.

8.2.1 Time Domain Specification

The time domain specification is used to set the peak amplitude excursions (about a stable ambient value) in time above which a test fails. Such features are desirable in site surveys, for example, as the acceptable signal level can be set in Spectramag-6 according to the allowable limits or according to the desired signal level in a test. This is an important time-saving feature given that a user is instantly notified of the failure of a test (at the point of detection). A decision can then be made whether to terminate a test or not or to restart a test, say at a new location. The maximum excursion is set by ticking the **Apply Time Domain Specification** checkbox and entering the desired value in an input box (**Figure 7**). The program detects both the positive and negative excursions from the ambient (zero signal) level.

8.2.2 Frequency Domain Specification

This feature is useful for specifying both the amplitude (rms) and the frequency of the component to be detected. Both the amplitude and frequency limits are also set using the dialogue box in **Figure 7**, by entering each frequency value and its corresponding amplitude value in the Frequency/Hz and Intensity/uT boxes respectively, and clicking the **Add** button.

Note: The autoscaling feature in Spectramag-6 will set the range of the plot according to the value entered for the Pass/Fail test. Hence it is good to have a fair idea of the magnitude of the signal to be detected.

Normally initial tests should be done with various small limits to gauge the size of the signal and the proper detection limits can then be set accordingly.

For example: if a limit of 2 μ T (2000nT) is set and the actual signal acquired/detected is 1nT, then the plot will look like a straight line due to the difference in magnitude. To see the measured signal, right-click the plot, select **Properties** → **Axis**, and set a smaller range e.g. 2nT.

Note: The values entered are listed as **Intensity/ μ T**, i.e. the entered values are assumed to be in μ T. Hence to detect a 10 μ T (rms) signal, simply enter '10' in the input box. Equally, to detect a signal of 50pT (rms) enter '50E-6' in the input box.

For effective detection, it is useful to set at least three other points of detection around the value of interest. For example, to detect a 16pTrms value at 50Hz, the following values can be set (as shown in **Figures 7 and 8**):

Freq	rms to be detected (pT)
48	46
49	16
50	16
51	16

The plot in **Figure 8** shows the outcome when the measured signal exceeds the set limit at 50Hz, at which point a failure was indicated. Notice that the limits set in **Figure 7** are in rms, hence rms should be selected [using a drop-down menu under the **FFT** sub-menu (**Figure 12**)] when displaying the results from the pass/fail tests so that the pass/fail results will also be in rms.

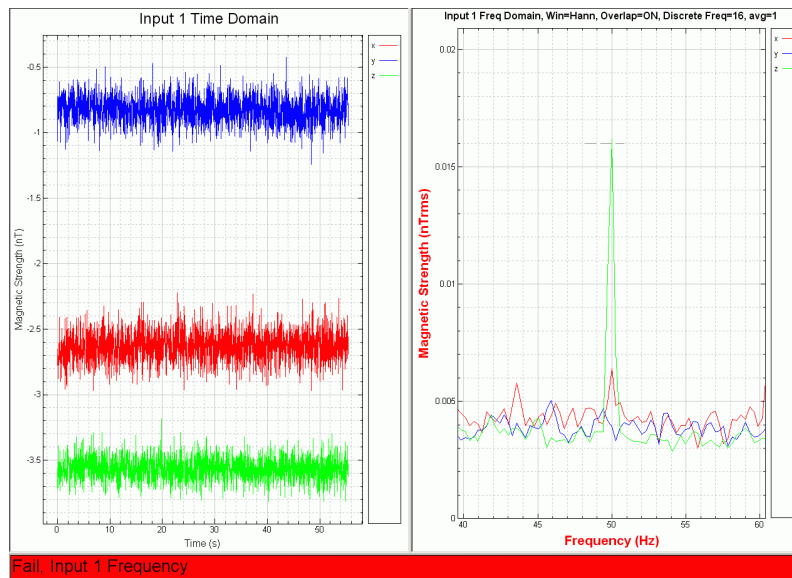


Figure 8: Test failure when the measured signal exceeds the set limits.

Note: When Time Domain or Frequency Domain Specification is used (and the Display Specific Curves option is selected), the auto-scale is disabled and the Maximum Excursion that the user specified is used as the plot range. If the range specified is much larger than the actual signal then one will only see straight lines. In that case the zoom option should be used by holding down the left mouse and dragging a box around an area of interest to zoom in. Alternatively a suitable excursion limit should be specified or the Display Specific Curve box should not be ticked.

8.3. Instrument Setup Sub-Menu

This sub-menu contains the controls for setting the gain for the magnetometer, accelerometer and microphone inputs as shown in **Figure 9**. The gain may be set to 1, 10, 100 or 1000.

Note: In normal circumstances a gain of 1 should be selected for magnetometer inputs, unless AC input coupling has been selected when a gain of 10 or more may be appropriate.

With a gain of greater than 1 and DC coupling selected, the DC levels due to the geomagnetic field may cause the input amplifiers to saturate.

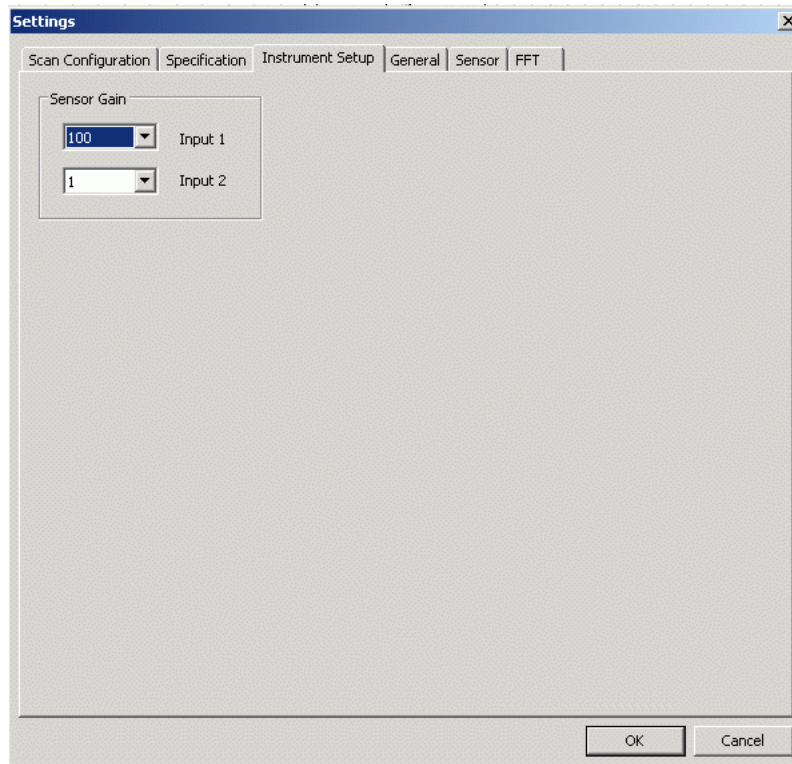


Figure 9: The Instrument Setup sub-menu.

As the accelerometer and microphone outputs contain no DC component, amplification may be applied without causing DC saturation of the amplifiers. For a 1V/g accelerometer, a gain of 100 is appropriate and for a 10V/g unit a gain of 10 is recommended.

Note: If a gain of 1000 is selected, the bandwidth of the Spectramag-6 input amplifiers will be reduced from 3.5kHz to about 1kHz (-3dB point). When a gain of greater than 1 is selected, the software applies an appropriate attenuation to compensate for the gain so the values displayed will remain constant at all gain settings. Therefore, if an AC field of 10nTrms is applied to a magnetometer then the signal will appear as 10nTrms on the display at all gain settings, and the operator does not need to consider the gain factor. The amplifiers are positioned before the A/D converter so gain may be used in critical applications to increase the signal-to-noise ratio, as the signal will be amplified while the internal noise of the A/D converter will not.

8.4. General Sub-Menu

This sub-menu (**Figure 10**) lets the user select the **Data Folder** where data can be exported after a scan is completed.

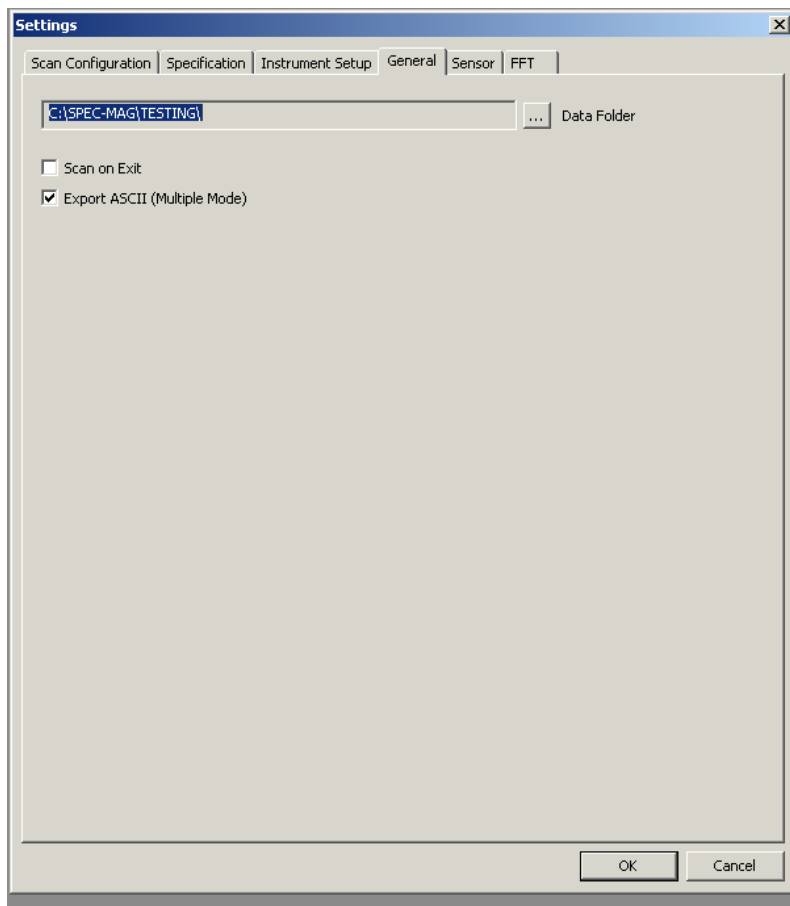


Figure 10: The General sub-menu.

The user can browse to a folder by clicking the ... button. For **Single** and **Continuous** acquisition modes, the data have to be manually saved on completion of a run (by clicking **File → Export → Data** and selecting the location and the name of the data file to be created) whereas in the **Multiple** mode the data is automatically saved to the specified location. The data is saved as a .sm6 file which contains the data, time and frequency domain plots and the settings used in a run. The **Multiple** mode also has the option of exporting data as ASCII files for use in spreadsheets such as Microsoft Excel or in other programs such as MATLAB.

The **Scan on Exit** box (if ticked) will cause an immediate scan when exiting the **Settings** menu by clicking the **OK** button. If it is not ticked, a run can be started by clicking **Scan → Run** in the toolbar or by clicking the green tick ✓ symbol. A 2-second delay (when DC coupled) or 10-second delay (when AC coupled) will be introduced before starting a scan, to allow the Spectramag-6 input filters to settle.

8.5. Sensor Sub-Menu

The **Sensor** sub-menu (**Figure 11**) allows a user to select their preferred units for magnetic field, vibration and sound measurements. In **Units** the options for magnetic field are nT, μ T and mGauss (mG) whilst the options for vibration are μ g, mg, g or mms^{-2} .

Note: Selecting these options will cause the graphics to be displayed in the appropriate units.

The unit for sound measurements is set to Pascal.

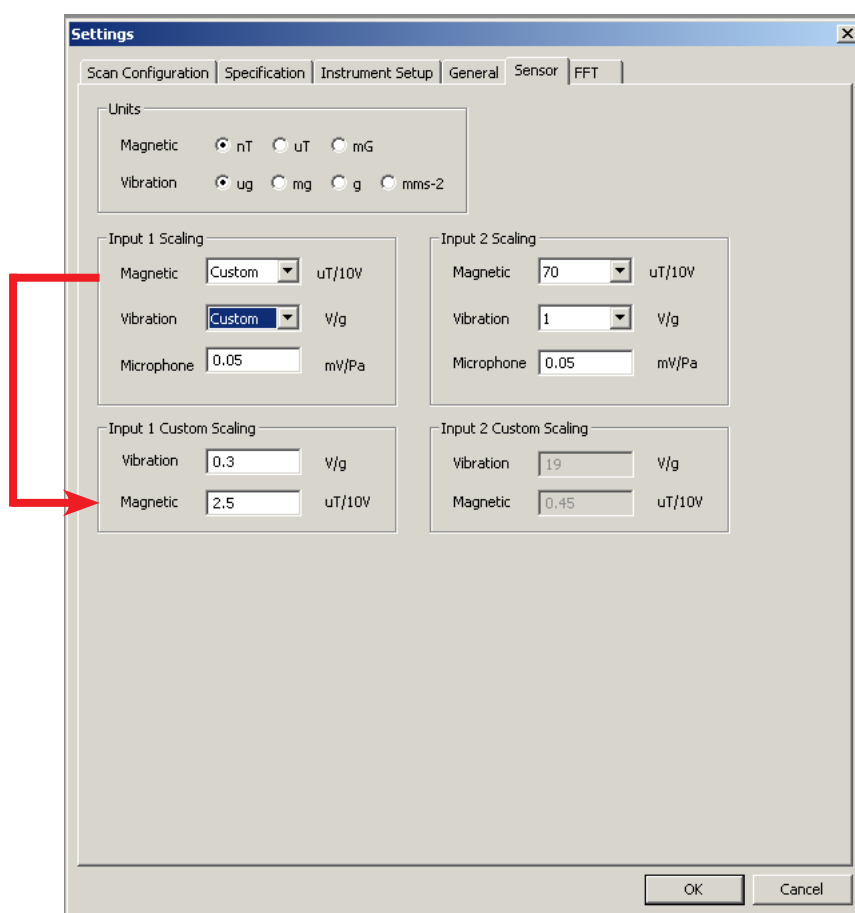


Figure 11: The Sensor sub-menu.

The **Input 1** and **Input 2 Scaling** settings allow the correct sensor scaling to be selected. The **Magnetic** scaling corresponds to the available range of Bartington Instruments' compatible sensors from $70\mu\text{T}/10\text{V}$ to $1000\mu\text{T}/10\text{V}$. There is also a Custom option that lets the user enter a custom magnetic scaling (in the Input 1 or Input 2 Custom Scaling boxes), as shown by the red arrow in **Figure 11**. The **Vibration** box allows the accelerometer scaling to be set to 1V/g , 10V/g or Custom. Similar to the **Magnetic** scaling, selecting the **Custom option** from the box activates **Input 1** or **Input 2 Custom Scaling** input boxes, letting a user enter custom scaling factors for the accelerometers connected to each input group of the Spectramag-6 unit. The microphone scaling is set via the **Microphone** input box and the value should be set (as a default) to 50mV/Pa to match the recommended microphone specification.

8.6. FFT Sub-Menu

Spectral analysis in Spectramag-6 is accomplished using a Fast Fourier Transform (FFT) algorithm. The spectral plots are produced during data acquisition, and when saved data are recalled and post-processed. The following are the key features for spectral analysis using the Spectramag-6 software.

8.6.1 FFT Windows

FFT windows are useful for minimising spectral leakage that causes power to leak from each spectral component to all other bins. The leakage from strong spectral components often completely swamps weaker components, making them hard to detect or resolve in frequency: hence FFT windows are extensively used for Fourier analyses. There are five FFT windows in Spectramag-6 (**Figure 12**) that can be selected, namely:

- Uniform (None) Window
- Bartlett Window
- Hamming Window
- Hann Window
- Welch Window.

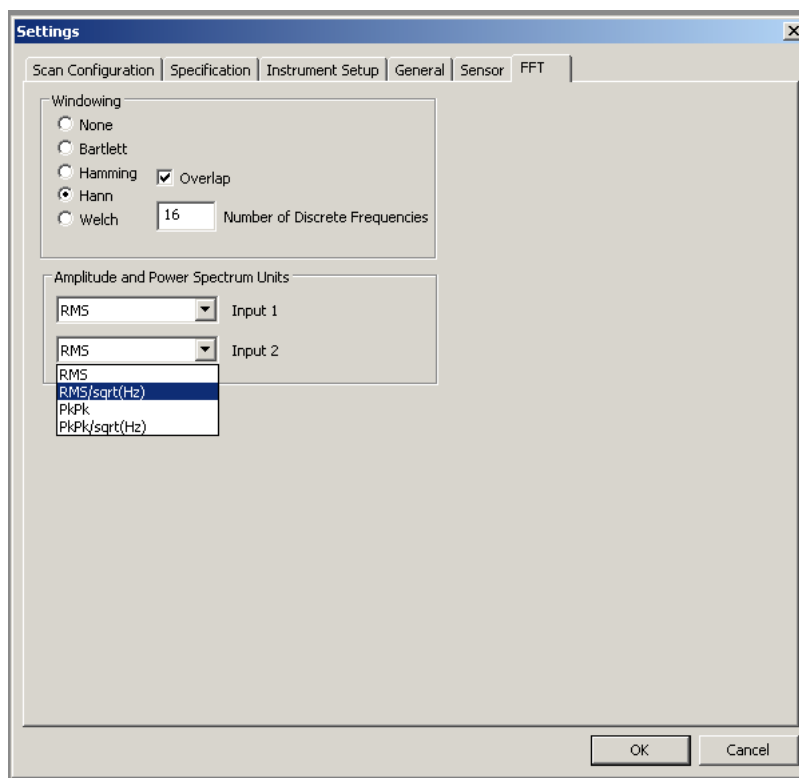


Figure 12: FFT settings for the Spectramag-6 software.

The choice of an FFT window depends mainly on the signal being processed, the desired amplitude accuracy and the required frequency resolution. For example, the Hamming window is suited to analysing closely spaced sinusoids and gives the best frequency resolution but not the optimal amplitude accuracy.

On the other hand, a Hann window is good for analysing narrowband random signals, combination of sinusoids or signals of unknown content. It gives slightly better amplitude accuracy but lesser frequency resolution compared to the Hamming window. Hence the choice of window depends on the signal being processed and whether the point of interest is signal detection or frequency resolution (see [Appendix B](#) for further details on FFT windows).

8.6.2. Overlap Processing

FFT windows reduce spectral leakage and improve frequency resolution by forcing both ends of an input waveform to zero or near to zero to avoid end-to-end mismatch. However this leads to data loss at both ends.

Note: Overlap processing is a method used to reduce such data loss by recovering the data normally eliminated by the tapering ends of FFT window functions. In overlap processing a longer data set (more than that required to produce a desired frequency resolution) is normally obtained. This data is then broken into segments which are overlapped, windowed and FFTed: the results are then combined. In Spectramag-6 the overlap feature can be selected by ticking a box as shown in Figure 12. The percentage overlap is fixed at 50%.

The other useful feature in the FFT sub-menu is the **Number of Discrete Frequencies (NDF)**. The NDF represents the number of segments that the data set is broken into and allows faster data processing by enabling smaller segments of data to be FFTed rather than processing a large chunk of data all at once. In Spectramag-6, NDF ranges from 1 to 16. The NDF is used in conjunction with overlap processing giving the following possible configurations:

- (i) Overlap ON, NDF (set from 1 –16).
- (ii) Overlap OFF, NDF (set from 1 –16.)

In (i) the acquired data is broken up into the number of segments set by NDF. Segments are overlapped, windowed and FFTed. In (ii) the acquired data is broken up into the number of segments set by NDF: these are each windowed and FFTed (without overlapping) and the results are then combined. In each case best results are obtained with NDF = 16.

Note: In order to use an NDF greater than 1, enough data **must** be acquired. This follows the formula:

$$\text{Data points required} = 4 * \text{NDF} * 1024$$

This is summarised in **Table 3**.

Table 3: The minimum number of data points required for each NDF

NDF	Minimum data points reqd.		NDF	Minimum data points reqd.
1	4096		9	36864
2	8192		10	40960
3	12288		11	45056
4	16384		12	49152
5	20480		13	53248
6	24576		14	57344
7	28672		15	61440
8	32768		16	65536

Note: For best performance, NDF used should also be a power of two

8.6.3. Spectrum Selection

The Spectramag-6 software produces two forms of outputs:

1. spectral amplitudes in rms and Peak to Peak
2. Amplitude Spectral Density (ASD) values in rms/√Hz and Peak to Peak per square-root-Hertz i.e. PkPk/√Hz.

Each option is selectable via a drop-down menu as shown in **Figure 12**.

These four options are available to all input types and measurements. For example, when a magnetometer is selected as the input source (**Figure 5**) and nanoTesla (nT) is selected as the unit (**Figure 11**), the output is displayed as nanoTesla-rms (i.e. nTrms) or nTrms/√Hz based on whether rms or rms/√Hz is selected in the drop-down menu in **Figure 12**. Similarly if the accelerometer is selected as the input source and the unit is set to microgravity (μg), then the output plot is displayed as μgrms or μgrms/√Hz based on whether rms or rms/√Hz is selected in **Figure 12**. Other units can be selected in a similar manner. **Table 4** shows more examples of how the units for the graphical plots are selected.

Table 4: Example showing how units for graphical plots are selected.

Input selected (Figure 6)	Units selected (Figure 11)	Spectrum selected from FFT sub-menu (Figure 12)	Unit used in plots
Magnetometer	μT	rms	μTrms
Magnetometer	μT	rms/√Hz	μTrms/√Hz
Magnetometer	nT	rms	nTrms
Magnetometer	nT	PkPk	nTPkPk

Accelerometer	μg	rms	μgrms
Accelerometer	μg	rms/VHz	$\mu\text{grms/VHz}$
Accelerometer	mms^{-2}	PkPk	$\text{mms}^{-2}\text{PkPk}$
Microphone	mV/Pa	rms	Parms
Microphone	mV/Pa	rms/VHz	Parms/VHz
Microphone	mV/Pa	PkPk	PaPkPk

9. Acquiring Data

After the desired settings have been selected, a scan can be initiated by selecting **Scan → Run** from the toolbar or by clicking the green tick ✓ symbol. If the **Scan on Exit** option is selected (from the **General** sub-menu) then a scan will also be initiated on selecting **OK** from the **Settings** menu.

When exiting from the **Settings** menu, a two-second delay will occur (if input coupling is set to DC) while the magnetometer zero offsets are calibrated. When an accelerometer, microphone or a magnetometer with AC input coupling is selected then the delay is increased to ten seconds to allow the input filters to settle. Depending on the signal level, a much longer settling time may be required when the highest resolution is needed. Repeated scans will show the filter settling with time.

During a scan, the progress can be observed at the bottom-right corner of the screen where the number of samples acquired and the number of averages or the number of runs completed are shown. If a time domain display was selected for any of the input groups then it will be shown and updated about once per second, but there might be a longer delay at low sample rates.

Note: If selected, the frequency domain plots will be displayed only on completion of a scan. If averaging has been selected, it will only be applied to the frequency domain display.

The time domain display is updated approximately once a second with the latest time data while the frequency domain display will be updated with the result of the latest average.

Note: The user's computer may become slow if too many scans are run and the files are left open. Save and close the files not required before running a new scan by doing **File → Close All**.

A typical Spectramag-6 plot is shown in **Figure 13**.

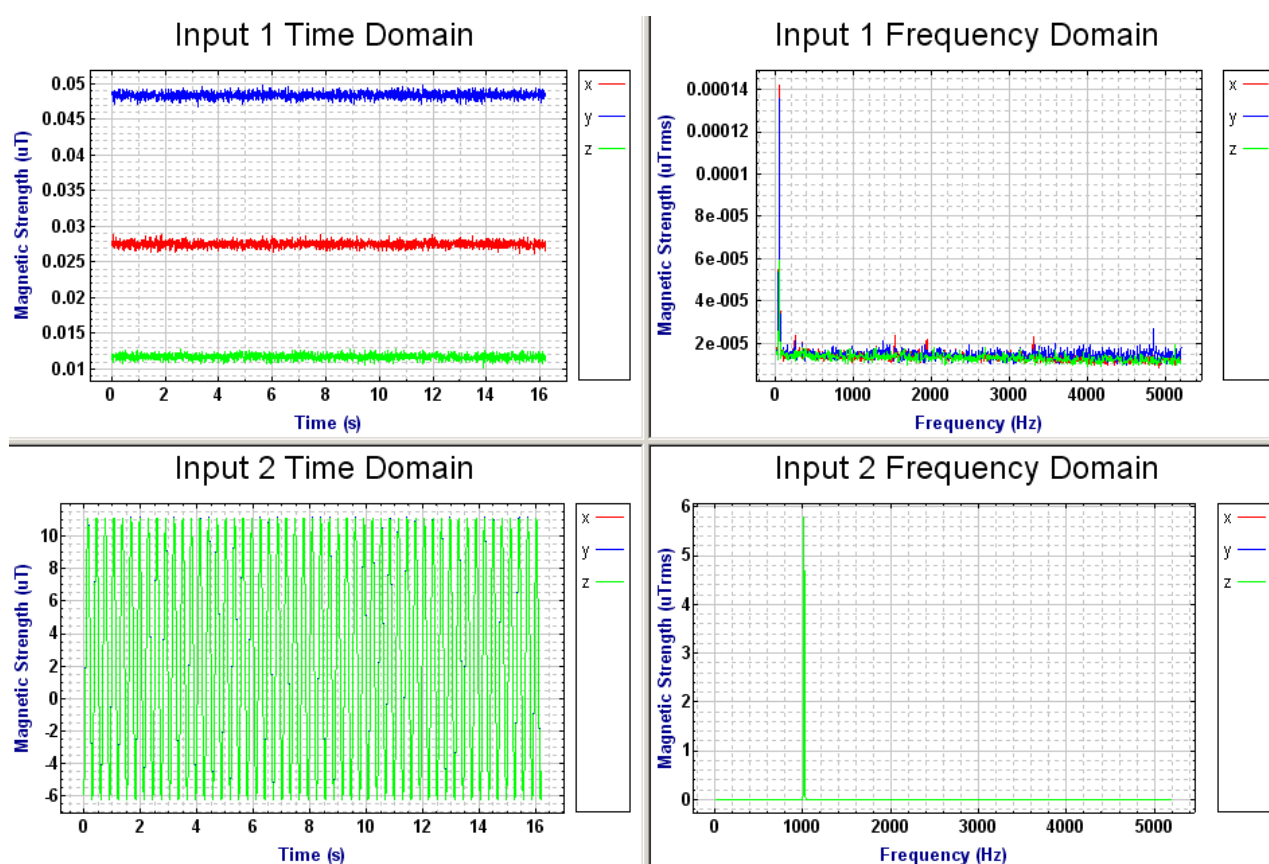


Figure 13: Time and Frequency Domain plots from Spectramag-6.

9.1. Quick Summary of Data Acquisition Using DC or AC Coupling

Note: Using the correct physical coupling between the Spectramag-6 system and the external sensors is crucial during data acquisition in order to ensure a high fidelity of the acquired signal.

Sensors can be AC or DC coupled to the Spectramag-6 system.

9.1.1. DC Coupling

DC coupling is useful for acquiring very slow varying signals (quasi-DC or DC). A gain of 1 is generally suggested to avoid the saturation of the input amplifiers in the Spectramag-6 unit that have output ranges of $\pm 10V$.

9.1.2. AC Coupling

AC coupling is required when there is a need to measure a small AC signal that requires amplification prior to signal acquisition. Very often the desired AC signal is superimposed on a large DC offset. If a gain is applied to such a signal, the DC offset will be large (after amplification) and may saturate the Spectramag-6's input amplifiers, which have a maximum output range of $\pm 10V$. By selecting **AC Coupling**, the DC offset is removed and a gain can then

be applied to the remaining AC signal. The gain setting to use depends on the magnitude of the signal to be acquired. It is typically from x10 to x100. If the input signal is a small AC and DC signal (say from a magnetometer) or purely an AC signal, then AC coupling should be used and a gain of >1 should be used to increase the overall signal-to noise ratio of the system (i.e. the ratio of the input signal relative to internal Spectramag-6's A/D converter noise).

9.1.3. Process of Data Acquisition

Note. When taking a succession of acquisitions with AC coupling, especially where the sensor(s) are moved in between acquisitions, the user must go through the settings window before each acquisition. This will force the stabilising input process, and prevent the introduction of errors in the measurements.

The process of data acquisition using DC or AC coupling in the Spectramag-6 software is shown in the following screen-shots Figures 14 (a) – (e) and explanatory notes.

(1) Switch the Spectramag-6 system ON and connect sensors to the input(s). Launch the Spectramag-6 software:

(i) Click the * sign on the software to see the **Settings** window as shown in **Figure 14a**.

(ii) Select which input to use and in the **Mode** box select the sensor to use, e.g. 'Magnetometer'.

(iii) Select DC in the **Coupling** box (if Accelerometer or Microphone is selected in (ii), the default is AC coupling and this box is greyed out).

(iv) Select **Both** to display both Time and Frequency plots, or select either Time or Frequency in the **Display Type** box.

(v) Select **Normal** in the **Display Mode** box. (Other options are **Mean-Zero** and **Offset-to-Zero**.)

(vi) Tick the **Autoscale** box to autoscale the plots or enter custom values in the Y Minimum and Y Maximum boxes.

(vii) Tick the **Low Pass** button to apply a Moving Average Lowpass filter to the time plot or select **None** if no filter should be applied. If Low Pass filter is selected, then enter the **Number of Rolling points** to be used in the Low Pass filter.

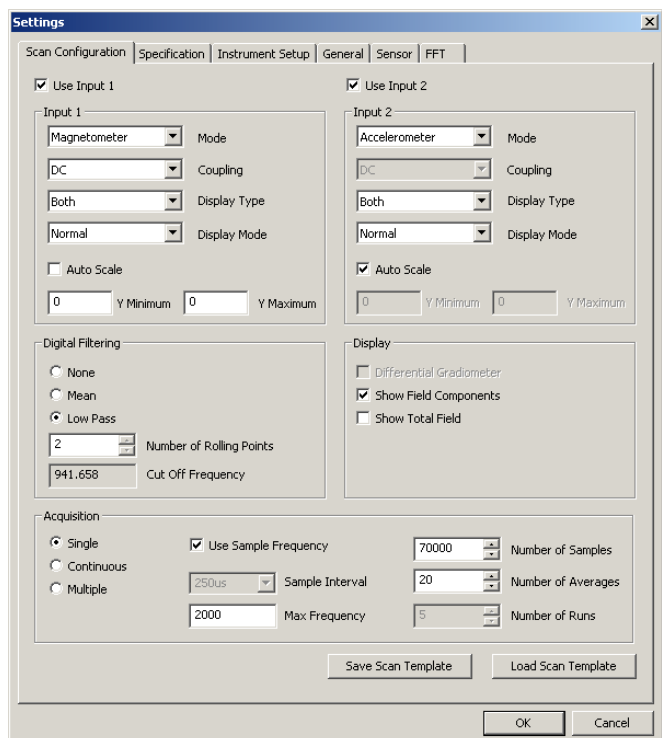


Figure 14a. Process of data acquisition.

(viii) Select **Single**, **Continuous** or **Multiple** acquisition mode (see [Setting Acquisition Modes](#)).

- If **Single** acquisition is selected: enter the No. of Samples and the No. of Averages.
- If **Continuous** is selected: enter the No. of Averages.
- If **Multiple** is selected: enter the No. of Samples and the No. of Runs.

(ix) Tick the **Use Sample Frequency** box and enter a value in the **Max Frequency** box: otherwise, enter the sampling period (1/f) to use. The **Max Frequency** value should be half the desired sampling frequency.

(2) The **Specification** sub-menu (**Figure 14b**) lets the user set the peak excursion of the input signal at which a test should fail.

To set values in the time domain, check the **Apply Time Domain Specification** and enter a value in the **Maximum Excursion** box. Values entered in the box are considered to be in μT . Hence if 7 is entered then the program will indicate a fail if a signal of up to $7\mu\text{T}$ is detected.

To set the values for the frequency domain:

(i) Select the **Apply Frequency Domain Specification**.

(ii) Enter a value in the **Frequency/Hz** and **Intensity/ μT** boxes and click **Add**.

Up to three values should be added very close to the value of interest. For example, to detect a $17\mu\text{T}$ peak at 100Hz, enter three values as shown in **Figure 14b**.

(iv) Check the Display Specification curves to see the excursion limits set, and click **OK**.

(3) In the **Instrument Setup** sub-menu (**Figure 14c**), set the gain to be applied to the two input groups labelled Input 1 and Input 2 of the Spectramag-6 system.

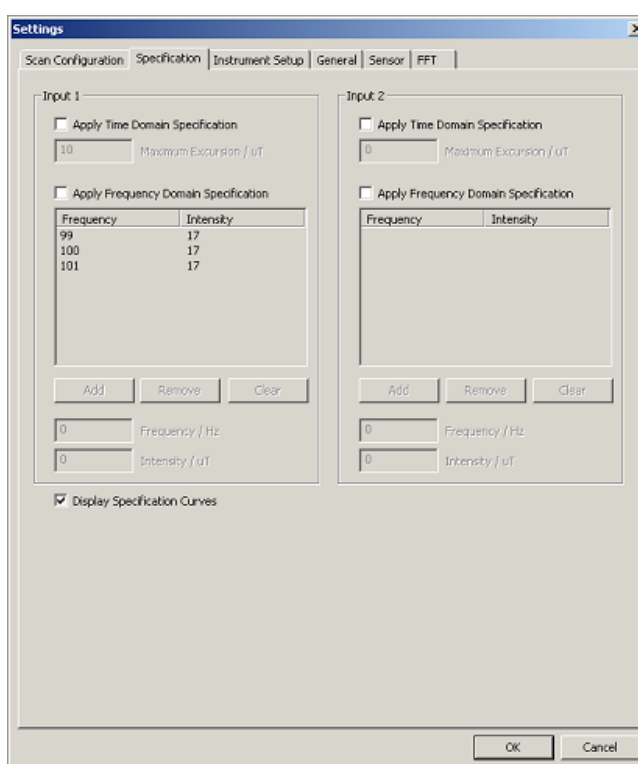


Figure 14b. Process of data acquisition.

Note: For DC coupling a gain of 1 should be used. Applying a gain (>1) with DC coupling can cause the Spectramag-6's input amplifiers to saturate if, for example, the background geomagnetic field exceeds $\pm 10\text{V}$ (i.e. the output voltage range of the Spectramag-6 input amplifiers).

(4) In the **General** sub-menu (**Figure 14d**):

(i) Set the location where the file is to be saved.

Note: Data is saved automatically in .sm6 format only when the **Multiple** mode is selected. Additional files are also saved automatically in ASCII format if the **Export ASCII option** is selected.

Note: For **Single** or **Continuous** mode, data can only be **manually saved**. To save all the plots and data for a Spectramag-6 scan, use **File → Save** or **Save As** options. To save only the data or plot, do **File → Export → Data** or **Export → Graphics**.

(ii) Tick the **Scan on Exit** box to have Spectramag-6 start a run once the **OK** button is clicked. Alternatively a scan can be initiated by selecting **Scan** and **Run** from the Spectramag-6 toolbar or by clicking the green tick ✓ symbol.

(iii) Tick the **Export ASCII** box to have scan data exported automatically to the specified location in ASCII format. This applies only to the **Multiple** acquisition mode which can be selected from the **Scan Configuration** menu.

(5) The **Sensor** sub-menu (**Figure 14d**) is broken into three groupings namely: (i) **Units** (ii) **Input Scaling** and (iii) **Custom Scaling**.

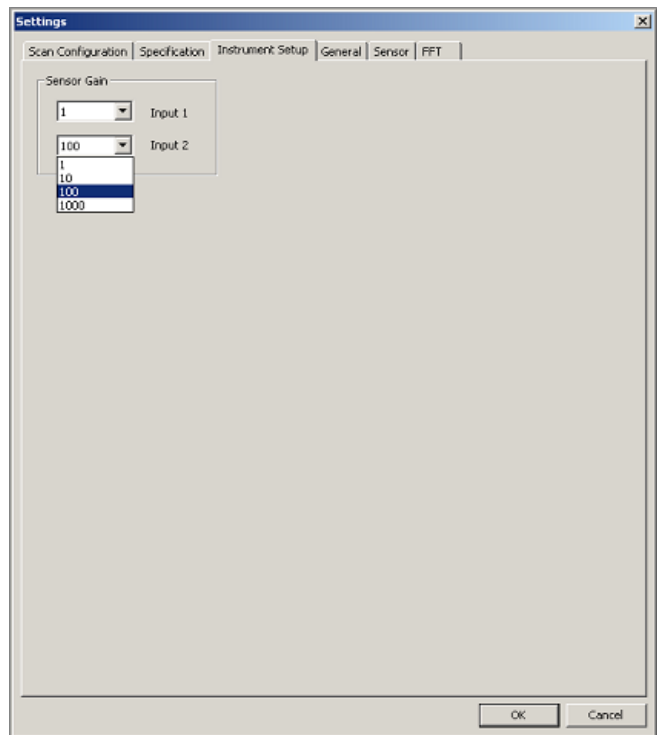


Figure 14c. Process of data acquisition.

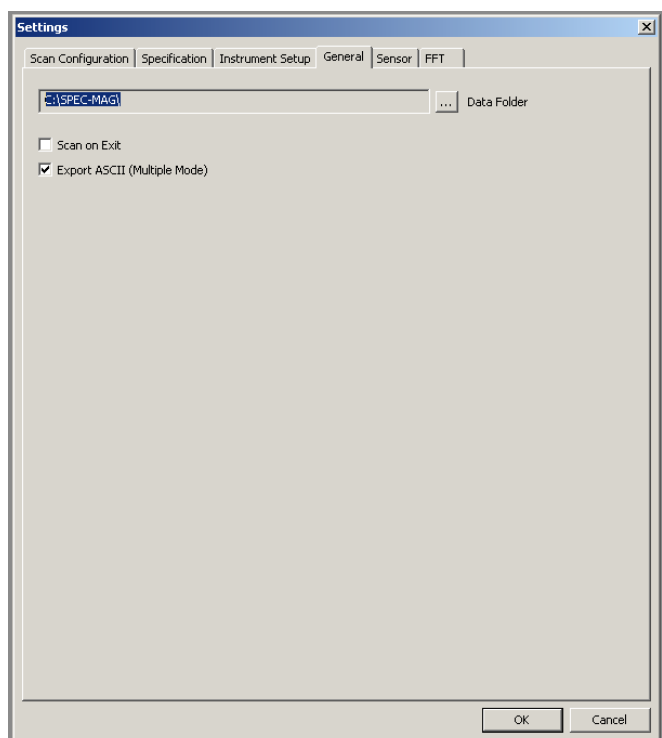


Figure 14d. Process of data acquisition.

(i) In the **Units** group, tick the units to be used for magnetic or vibration measurements. **These settings apply to both Input 1 and 2.** Selecting these options causes the plots to be displayed in the chosen units.

(ii) In the **Input Scaling** group select the scaling factor for the Magnetic or the Vibration sensors or the Microphone.

The **Magnetic** scaling corresponds to the available range of Bartington Instruments' sensors from $70\mu\text{T}/10\text{V}$ to $1000\mu\text{T}/10\text{V}$. Selecting **Custom** from the box activates the **Magnetic** text box under the **Input 1** or **Input 2 Custom Scaling**. This enables a user to enter custom scaling factors to use with a magnetometer.

(iii) The **Vibration** box allows the accelerometer scaling to be set to 1V/g , 10V/g or **Custom**. Selecting **Custom** from the box activates **Input 1** and **Input 2 Custom Scaling** input boxes, enabling a user to enter custom scaling factors for an accelerometer.

(iv) The Microphone text box allows a custom scaling factor to be specified for a given microphone input.

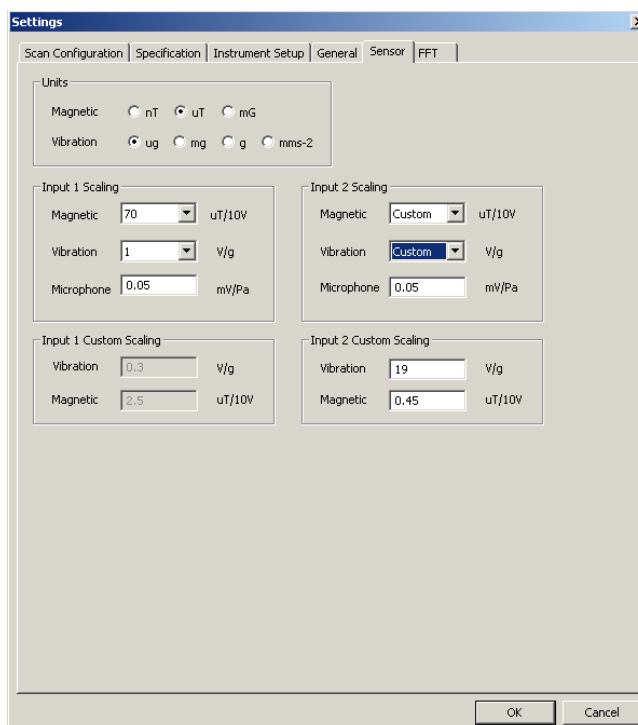


Figure 14e. Process of data acquisition.

(6) In the **FFT** sub-section (**Figure 14e**) are various windows that can be applied to a data before being Fourier Transformed. Select a suitable window. (See [FFT Windows](#) and [Appendix B](#) for further information.)

Tick the **Overlap** box and set **Number of Discrete Frequencies (NDF)** to 16.

Note: Enough data points **must** be acquired during a scan in order to use the NDF feature as shown previously in **Table 3**. So for $\text{NDF} = 16$, acquire a minimum of 65536 data points during any run.

10. Viewing Data and Annotating Displays

When a scan has been completed, the plotted data will be shown and the status at the bottom of the screen will show the unit to be in the idle state (**Figure 15**). The display type selection may be changed using the **View** menu item to select or deselect **Time** or **Frequency** for each input group. In this way one or all displays can be shown, or hidden and later retrieved.

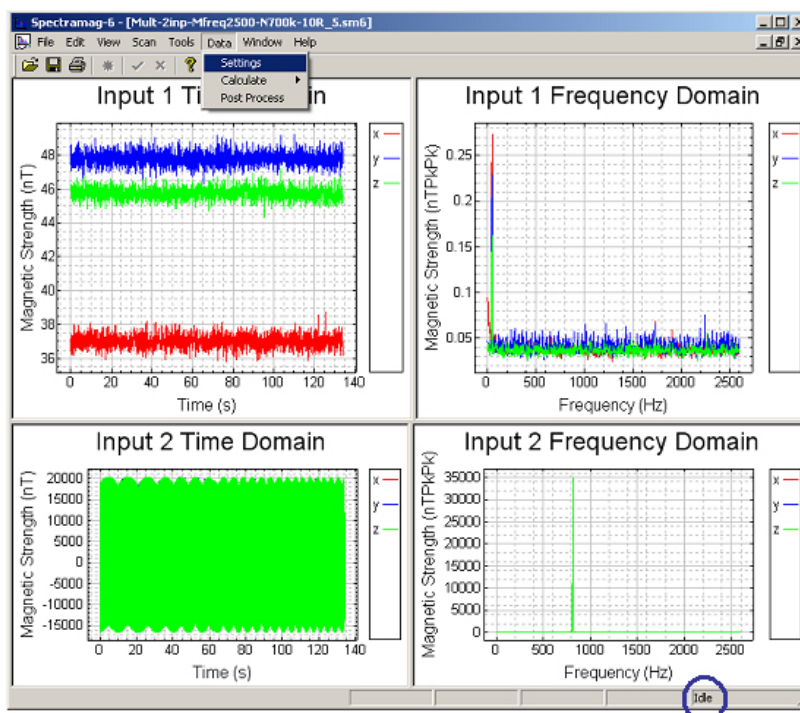


Figure 15: Changing the display modes.

The time domain display mode can be changed (after collecting the data) by selecting **Data** from the toolbar and then selecting **Settings**. A **Settings** menu will be displayed, allowing the time domain display to be switched between **Normal**, **Mean Zero** and **Offset to Zero**. The sensor units, scaling, display and the FFT settings can also be modified. These changes will be reflected in both the time and frequency domain graphs. If data has been acquired from a microphone, selecting **Data** and **Calculate** from the toolbar will allow the mean sound intensity over the frequency range to be displayed.

The following operations can also be carried out on each display window by clicking the mouse cursor within the selected window.

10.1. Zoom Control

If the cursor is moved to one of the display windows and the left mouse button held down, the mouse can be moved to select an area of the graph to be expanded. The scaling will be expanded with the graph, allowing accurate measurements to be made over a small section of the original display. The process may be repeated several times. To restore the display to the original state, click the right mouse button on the display and select **Show All**.

When many plots are shown as in **Figure 16**, the size of each plot can also be adjusted by dragging the borders of the plot.

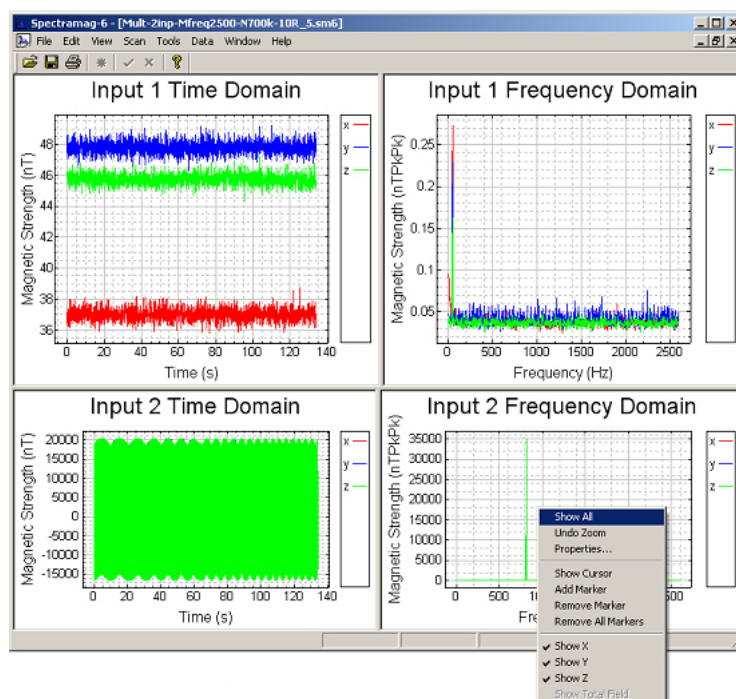


Figure 16: Spectramag-6 plot settings.

10.2. Plot Settings

If the mouse cursor is moved over one of the plots and the right button is clicked, a menu will appear offering **Show All**, **Undo Zoom**, **Properties**, **Show Cursor**, **Add Marker**, **Remove Marker**, **Remove All Markers**, **Show X**, **Show Y**, **Show Z** and **Show Total Field**. After zooming, **Undo Zoom** removes the effect of the last zoom action. When changes are made to the view, e.g. by a series of zoom actions, **Show All** resets the plot to the original state.

10.3. Plot Options

Selecting the **Properties** item (after right-clicking a plot) opens a new window called **Plot Options**. The **Plot Options** window has nine sub-menus (**Figure 17**) that allow additional control of plots such as setting plot titles, fonts, plot scales etc. Many of these functions will be reset to the default values when the program is restarted. To see the full range of sub-menus, use the left and right arrows (◀ ▶) at the top right corner of the main **Plot Options** menu.

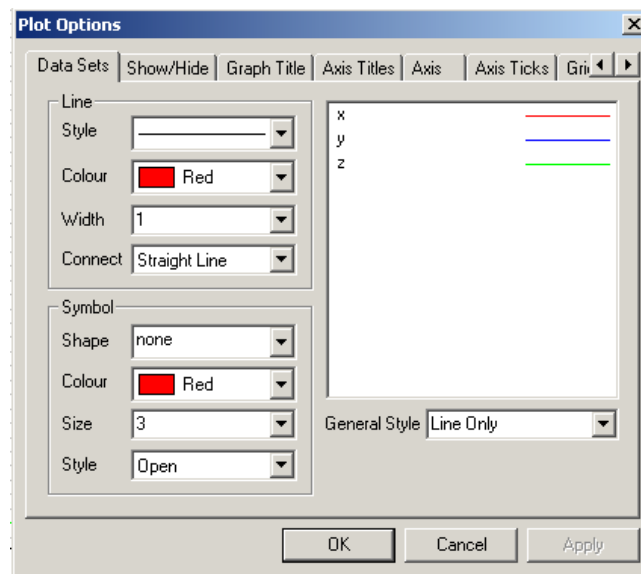


Figure 17: Changing plot parameters.

10.3.1. Data Sets

This sub-menu allows the lines and the symbols for each of the three axes on the plot to be selected from a range of styles, colours and sizes. The default settings give three narrow straight lines in red, blue, green and yellow lines (with no symbols) for the X, Y, Z and total field respectively. To change the line properties for each axis, click on the line on the right-hand side of **Figure 17** and select the properties from the settings on the left-hand side.

10.3.2. Show/Hide

This sub-menu allows the plot for each axis to be shown or hidden, enabling the three axes to be viewed individually or together.

10.3.3. Graph Title

The graph title can be edited in this menu to customise the plots for export to reports. Full control of fonts, text sizes etc. is provided.

10.3.4. Axis Titles

This sub-menu allows the X and Y axes titles' font types, sizes etc. to be changed.

10.3.5. Axis

The **Axis** sub-menu allows the axes scales to be set to linear or logarithmic. The user can also input the range of the X or Y axis, or both. Note that the program zooms into the plot when the log scale is selected. Use **Show All** to see the entire plot if required.

10.3.6. Axis Tick

Use the **Axis Tick** to set the major and minor tick marks for both X and Y axes. The font type, font size and the colour of the labels can also be set from this sub-menu.

10.3.7. Grid Lines

The major and minor gridline styles can be selected from this sub-menu. The user can also select different styles, colours and thickness of the grid lines.

10.3.8. Key

The **Key** sub-menu allows the legend to the X, Y and Z axes to be shown or hidden. The font types, sizes and the colours of the legends can also be changed in this sub-menu.

10.3.9. Cursors

The **Cursors** sub-menu lets the user select two cursors that can be used for measurements for each plot. Each cursor may be selected to be visible or not and associated with either the X, Y or Z axis.

10.4. Show Cursor

Clicking **Show Cursor** will cause a cursor to appear at the left edge of the plot. This may be moved horizontally across the plot by dragging with the mouse to a point of interest or by using the left-right arrow keys (◀ ▶). When a cursor is moved to any point, it gives the X and Y values of the signal at that point. For example, if a cursor is shown for a frequency plot, then the cursor gives the frequency and the amplitude of the signal as shown in **Figure 18**. This enables accurate readout of the values of the acquired signals.

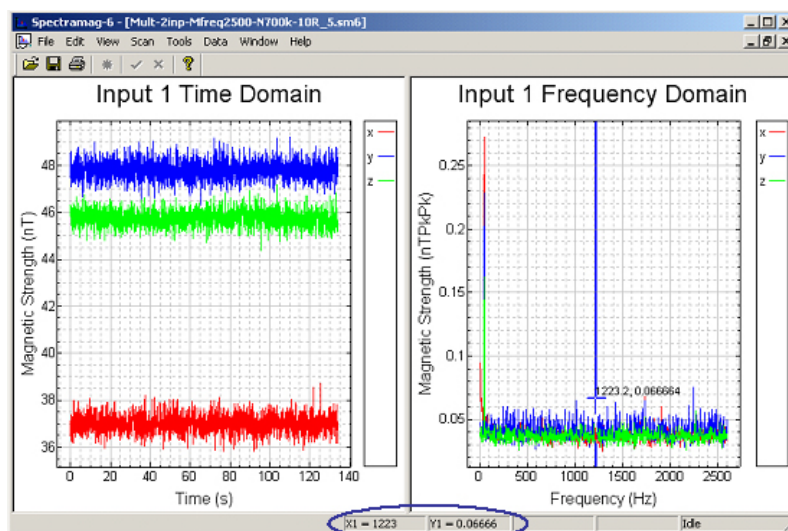


Figure 18: Using cursors in Spectramag-6.

To read out the values for any signal, use the up-down arrow keys (▲ ▼) to switch from the X to Y or to the Z signal cursor. The cursor will change colour to the corresponding colour of each

signal as the up-down arrow is pressed. If the plot resolution is too coarse then the cursor can be left in the region of interest and the zoom facility used to show the detail. The cursor may then be positioned with a greater accuracy.

Add Marker (Figure 16) causes a marker to be added to a plot at the position of the cursor. It also shows the X and Y values. The cursor may then be moved to another point, or may be removed by clicking on the **Show Cursor** option again. Markers may be removed using **Remove Marker** option. This causes the markers to be removed sequentially starting with the most recent. The **Remove All Markers** option clears all the markers from the current display.

The **Show X, Y, Z** and **Total Field** menu items (**Figure 16**) allow the individual axes to be added or removed from the plot by clicking the appropriate line. This allows an individual axis to be viewed and analysed during and after data acquisition.

11. Saving and Closing Files

For **Single** or **Continuous** acquisition modes, data can be saved in Spectramag-6 format (*.sm6) for subsequent retrieval, processing and display using the **File → Save** or **Save As** options. A single file or all open files may be closed without saving using **File → Close** or **File → Close All**. If a file is being closed by clicking the **Close** tab on the top right-hand corner of the Windows toolbar, the Spectramag-6 software will prompt the user to save each file before closing it. It is good practice to close files when not required as a large number of open files can slow down the program.

For **Multiple** acquisition mode, data is automatically saved as .sm6 files. Data can also be saved as ASCII files (in addition to the .sm6 files) if the **Export ASCII** option is ticked in the **General** sub-menu (**Figure 10**).

12. Exporting Results

When a file is open, it may be formatted for export to other Windows-based applications. Selecting **File → Export** gives the option of **Graphics** or **Data**. Selecting **Graphics** will show a list of the plots available. Click on the relevant plot and select **Continue**. This will produce a **Save As** menu where the folder and file name can be chosen and the file type selected as a Bitmap, JPEG or TIFF. When **OK** is selected, the image size can be set, the default size being 400 x 600 pixels. Graphics will be exported complete with any markers applied. These files may be readily imported into other applications to produce reports.

Data files are formatted as tab-delimited lines of data with a header showing the starting date and time of a scan from the computer's clock. The data headings are shown as time in seconds (from the start of a scan) and as the units selected by the user for the X, Y and Z axes. These files may be directly imported into applications such as Microsoft Excel, MATLAB etc. As mentioned

previously, for **Multiple** acquisition mode, data is automatically saved as .sm6 files and data can also be saved as ASCII files (in addition to the .sm6 files) if the **Export ASCII** option is selected.

Note: Ensure that enough storage space is available on the hard disk before using the **Multiple** acquisition mode, especially when acquiring large amount of data. Typically each Spectramag-6 file (with 700,000 points) is approximately 87Mb. Each ASCII (.dat) file with 700,000 data points is approximately 48Mb.

Graphics and data files can also be copied and pasted directly into other applications from the toolbar using **Edit → Copy**.

13. Data Recall and Processing

During data acquisition in Spectramag-6, a pre-filter can be selected enabling certain frequencies to be removed from the acquired data prior to it being displayed (see [Digital Filtering](#)). Additionally, the Spectramag-6 software provides a post-processing feature (**Figure 19**) for use when data is acquired without filtering and additional processing is required. This enables a user to recall and post-process the acquired data in the following ways:

1. Averaging N number of files and displaying the final results.
2. Applying a Moving Average low-pass filter to any of the acquired data files. This feature is especially useful for filtering out power frequencies and their harmonics, e.g. in cases where the features of interest are the DC trends inherent in the acquired signal. This is often the case for data acquired in a noisy environment with substantial interference from 50Hz or 60Hz power line frequencies or their harmonics.

To post-process the acquired data:

1. Click **Data → Post Process** from the Spectramag-6 toolbar (**Figure 19**).



Figure 19: The post processing feature in the Spectramag-6 toolbar.

This opens a window allowing the user to select the file(s) to be processed.

2. To select a file or files, click on one file and then hold down the Control (CTRL) key and select the rest of the files to process. Click **Open**.

3. The selected files open, showing the **Post Processing** window as in **Figure 20**.

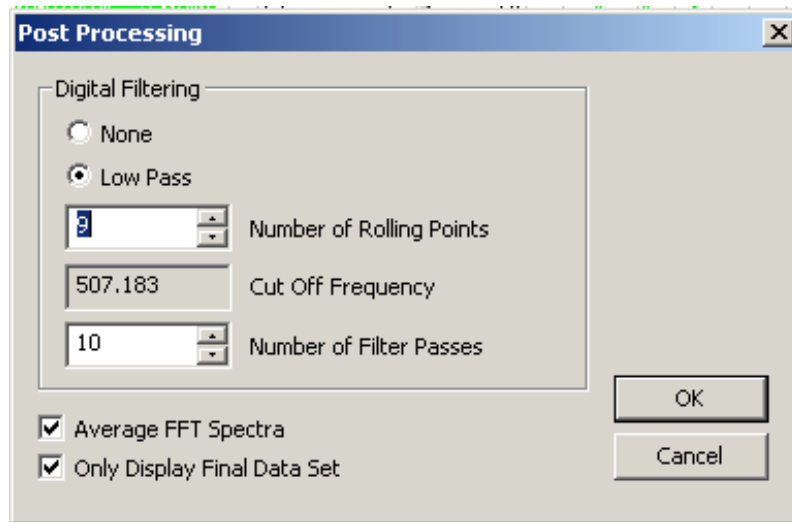


Figure 20: The Spectramag-6 Post Processing window.

The Post Processing window is in two parts: (a) Digital Filtering section and (b) Average FFT Spectra section. These are discussed in the following sub-sections.

13.1. Digital Filtering

Under the **Digital Filtering** section the user can select/deselect the post processing low-pass filter using the '**None**' or '**Low Pass**' button. When a filter is selected, the Number of Rolling Points (NRP) determines the number of points in the data that is averaged to produce the filter effect. Adjusting the NRP also sets the cut-off frequency of the filter. The Number of Filter Passes (NFP) affects the roll-off rate of the filter. For $NFP = 1$ one, the filter is applied once to the data. With $NFP > 1$ (say, $NFP = k$) the data is passed recursively k times through the filter. This is similar to passing the data through a cascade of k identical filters, leading to a steeper roll-off rate. **Figure 21** shows data before and after applying a filter.

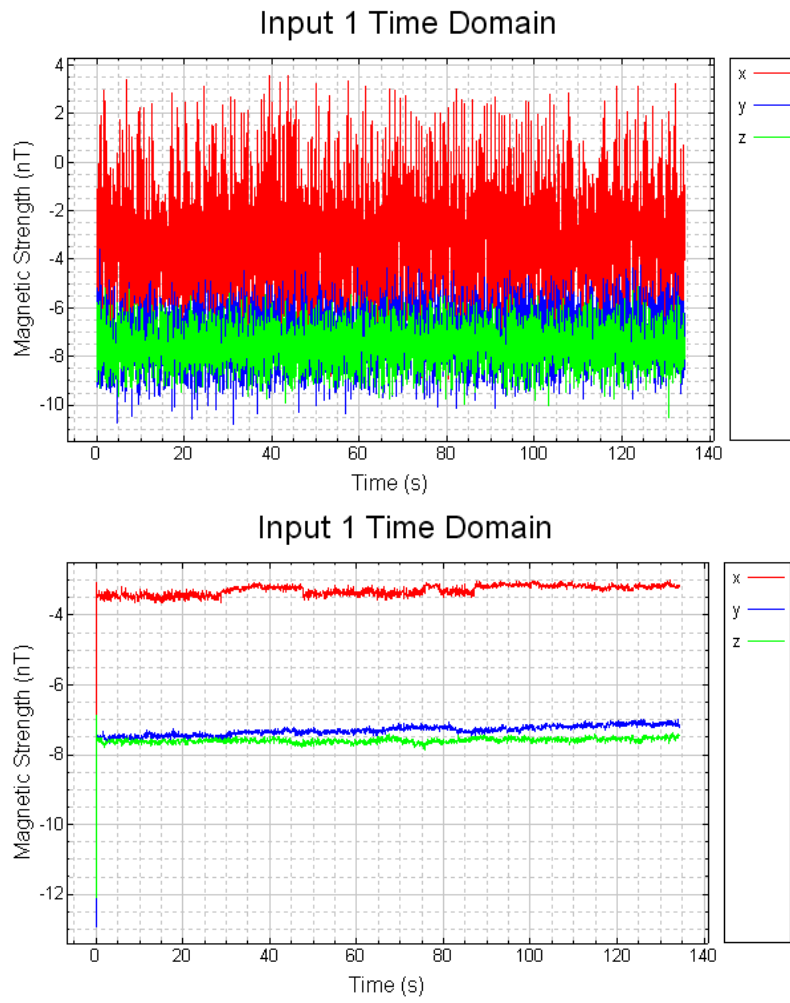


Figure 21: (a) Data acquired in a noisy environment and (b) the data after low-pass filtering.

13.2. Averaging FFT Spectrum

The Average FFT Spectra box (when selected) causes the Spectramag-6 program to produce the average of the N Spectramag-6 (.sm6) files selected by the user. The example in **Figure 22** shows two signals (a) and (b) and the result after averaging in (c).

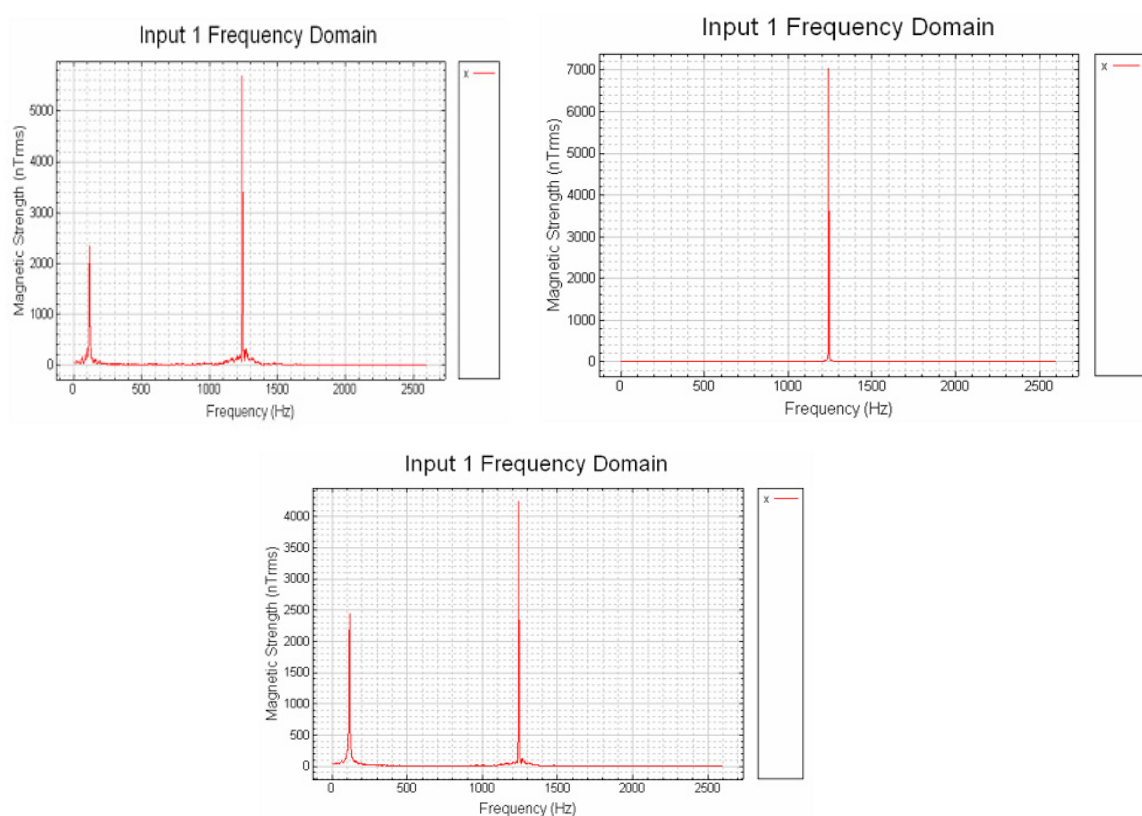


Figure 22: Signals from two logged data files (a) and (b), and the result (c) of averaging the two signals using the post processing Average FFT Spectra feature.

13.3. Only Display Final Data Set

This option is ticked to prevent many windows opening up when many files are post-processed in Spectramag-6. Ordinarily, when N files are selected for post processing, these files will open up in N different windows, but as many files can cause the software to become slow it is preferable not to open all the N files. By selecting the **Only Display Final Data Set** option, only the final window will be opened showing (for example) the average of the N files.

Note: In normal use, the **Only Display Final Data Set** should always be ticked so that only the final result of data averaging or filtering can be seen.

For limited number of files (≤ 20) the **Only Display Final Data Set** can be deselected. To see the opened N files, click the 'Restore Down'  symbol in the Windows toolbar. With N files open, the user can browse through the files to see the evolution of the time data or the frequency

components in the frequency domain as shown in **Figure 23**. These mimic the Joint-Time Fourier Analysis, e.g. the Short Time Fourier Transform (STFT) analysis where successive Fourier transforms are stacked in time.

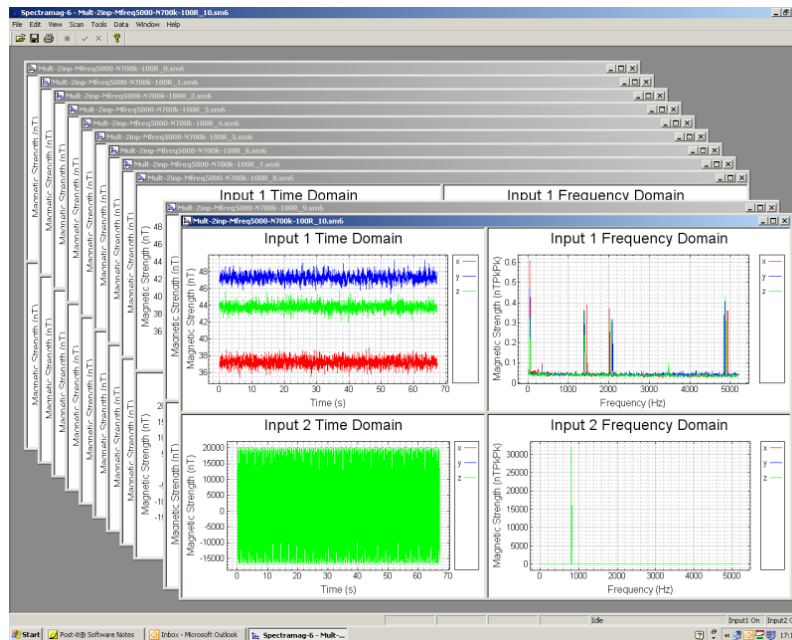


Figure 23: Opening multiple windows in the Spectramag-6 software.

14. Operating Practice

If an accelerometer or microphone or a magnetometer (with AC coupling) has been selected as the input device, a 10-second delay will be applied to allow the internal filters to settle.

Note: In order to obtain the best results, allow a few minutes for the system to warm up and the filters to settle before data acquisition.

The magnetometers are powered whenever connected to the Spectramag-6 unit but the ICP interface is powered down when accelerometers are not selected for input.

Note: When closing down, close the Spectramag-6 program before disconnecting the USB cable and then switch off the Spectramag-6 unit. Always ensure that the unit has been switched OFF before packing it away to avoid completely discharging the battery.

15. Interpretation of Results

In common with all data acquisition systems and spectrum analysers, care should be taken in interpreting the results obtained. The time domain display resolution may be much less than the number of data points used in a scan and aliasing may therefore occur. This is exactly analogous to under sampling and may cause some signals to appear at much lower frequencies than the

original signal. Using the zoom control allows a small increment of time to be expanded and the true frequency to be seen.

If either the time domain or the frequency domain display appears to show values much smaller than the full-scale range, then it is likely that the maximum rms value is not visible due to the pixel resolution of the display. This may happen if the number of samples is large and the spectral band or the peak signal is narrow. In order to find the maximum values under these circumstances, the zoom control should be used to check sections of the spectrum, giving a full resolution to the section of the spectrum selected. It is normally better to start with a relatively small number of samples to give an estimate of the maximum rms value and then increase the number of samples to improve the frequency resolution.

If the spectrum of an accelerometer has high levels at low frequencies, then it may be due to the DC offset of the accelerometer amplifiers. Select **Mean Zero** or **Offset to Zero** for the **Display Mode** to remove any DC component.

16. Troubleshooting

The system works reliably but bad data can be collected if the USB interface is interrupted or initially connected when the Spectramag-6 unit is not switched ON.

To restore correct operation:

- close the Spectramag-6 program
- disconnect the USB cable
- switch the Spectramag-6 unit off for a few seconds
- power it up again
- connect the USB cable and wait 10–15 seconds before restarting the program.

Bad data may also result from a low battery voltage. If the battery indicator (next to the ON/OFF switch) is amber or red then the battery should be charged before use. Additionally, bad data are also acquired if the complete system (PC, Spectramag-6 unit, sensors e.g. magnetometers) is connected up and the Spectramag-6 software is run without switching on the Spectramag-6 unit.

Note: see also [Important Points to Note Before Using the Spectramag-6](#).

17. Maintenance

The Spectramag-6 unit requires no routine maintenance. Re-calibration of the system by Bartington Instruments is recommended at two-yearly intervals.

17.1 Changing the Battery

The rechargeable Lithium Ion battery needs to be recharged periodically, even if the unit is not in use, and will last for approximately 300 charge/discharge cycles. A new battery should be fitted every 4 years.

Customers can replace the battery themselves, or it can be done by Bartington Instruments every other time that the system is returned as part of its regular service and calibration.

To gain access to the battery, remove the four screws securing the back panel with a 3mm hexagonal Allen key. The battery and all internal circuitry are contained in a single assembly tray with the battery clamped on top. Carefully pull out the assembly tray (**Figure 24a**) until the battery can be seen on the top of the assembly as shown in **Figure 24b**.

Note: Care must be taken to avoid stressing internal cables secured to the front panel.

The battery has an indicator showing the state of charge, activated by pressing the button below the indicator.



Figure 24a: Internal battery location.

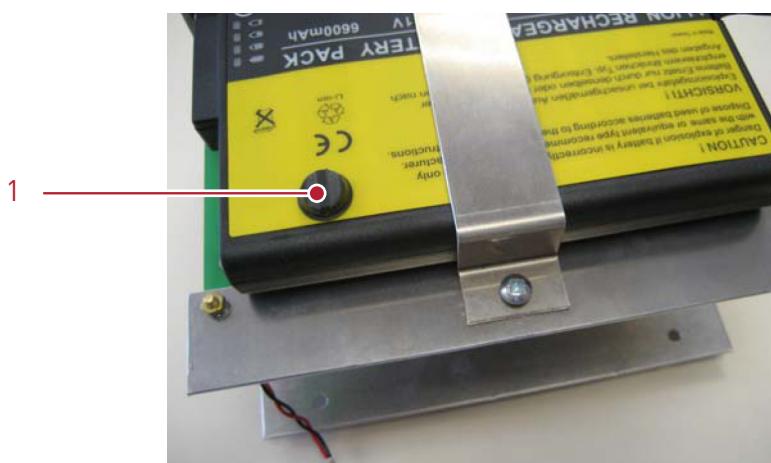


Figure 24b: Battery clamped to top of assembly, with rubber foot attached. [1]

To remove the battery, undo the two screws securing the clamp (**Figure 24b**) and carefully withdraw the battery from the connector on the circuit board. To replace the battery, reverse the above procedure.

Note: As shown in **Figure 24b**, fit a rubber foot on the top of the battery to prevent vibrations inside the enclosure when assembled.

17.2. Shipping the Battery in this Equipment

Batteries and equipment containing batteries should only be shipped in accordance with local regulations. Refer to the IATA website (www.iata.org) for regulations regarding air transport.



Caution: If there is any doubt at all as to the integrity of a battery – for example, cracked or dented casing – then it must not be shipped. Remove it from the equipment and dispose of it according to local regulations.

When changing batteries in this equipment, ensure that the replacement battery is of the same type as shown in its brochure, available on the product page.

Appendix A

A.1. Spectramag-6 Frequently Asked Questions (FAQ)

A.1.1. Sampling

How do I set the Sampling Frequency?

The sampling frequency is set in two ways. Firstly, when the **Use Sample Frequency** box is ticked, values can be entered into the **Max Frequency** box. This represents the Nyquist frequency. Note that the sampling frequency is twice the value entered for the **Max Frequency**. Secondly, if the **Use Sample Frequency** box is not ticked, the **Sample Interval** box is then activated from where a sampling period ($T = 1/f$) value can be chosen, ranging from 100 μ S to 10S. Note that for most systems it is recommended to use 10kS/s (max) for Single mode acquisition and 5kS/s (max) for Multiple mode acquisition.

How fast should I sample?

To properly represent and analyse a signal whose highest frequency component is f Hz, the signal should be sampled at a minimum of $2f$ samples/second according to the Nyquist sampling criterion, in order to avoid aliasing. Sampling a signal at twice its maximum frequency ensures that a signal can be properly reconstructed (after processing) and that its frequency can be accurately resolved. However, the Nyquist rate does not guarantee the accurate representation of the signal's shape or amplitude. To better capture the shape and amplitude of a signal, it should be sampled (as a rule of thumb) at ten times the Nyquist rate, i.e. at $20f$ samples per second.

How long will each run take?

The duration of a run (in seconds) on Spectramag-6 is obtained by **Equation 1**. Note that this time will vary slightly if say other programs are also running on the computer. It is advisable to close all the other programs before running Spectramag-6.

$$\text{Duration of a run} = \frac{\text{No of samples} * n}{2 * \text{Max Frequency}} \quad (1)$$

Where:

- Duration of a run is in seconds
- n is the number of averages or number of runs set in Spectramag-6
- Max Frequency is the maximum frequency value set in Spectramag-6

How much acquisition time do I get when I use a sampling frequency of fHz?

The acquisition time for a sampling frequency of fHz (where fHz = 2*Mx Frequency) is given by **Equation 2**:

$$\text{Acquisition time} = \frac{\text{No of samples}}{2 * \text{Max Frequency} \times N} \times N \quad (2)$$

Where:

- N = number of runs

Note that the total acquisition time is not shown on the time domain window as Spectramag-6 only displays the last scan. It is only shown for the Continuous Acquisition mode (see [Setting Acquisition Modes](#)).

How do I set the resolution of a frequency plot?

The frequency resolution determines the line width or the width of the FFT bins and is useful for setting the level of details (resolution) that can be seen on the frequency scale. For each analysis, consideration should be given to the frequency range and the resolution required as there is a trade-off between the frequency range/bandwidth and the corresponding frequency resolution. In Spectramag-6 the frequency resolution is given as **Equation 3**.

$$\text{Freq Resolution } (\Delta f) = \frac{f_{\text{samp}}}{2048} \quad (3)$$

Where

- f_{samp} = Sampling frequency

For example if the sampling frequency $f_{\text{samp}} = 102.4\text{Hz}$, $\Delta f = 0.05\text{Hz}$ and the range is from 0.05Hz to 51.2Hz, then as Spectramag-6 always starts plotting from the second point, the range would be from 0.1Hz to 51.2Hz as shown in Figure A.1 (a).

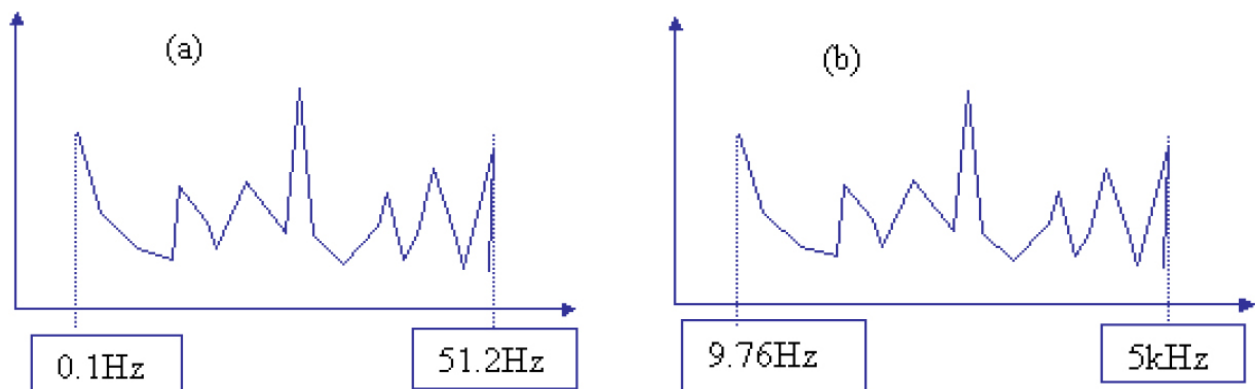


Figure A.1: A diagram illustrating how the resolution of a frequency plot can be chosen.

Similarly if a maximum frequency of 5kHz (i.e. $f_{\text{samp}} = 10\text{kHz}$) is selected, the frequency resolution or line width would be 4.88Hz per bin or per line on the FFT plot, giving a plot ranging from 9.76Hz–5kHz at 4.88Hz per bin (**Fig A.1b**).

Note: Be aware that the –3dB point of the Spectramag-6 system (and the frequency plots) is at 3.5kHz, or at 1kHz if an input gain of 1000 is selected in Spectramag-6.

What does ‘Max Frequency’ as shown on the Spectramag-6 software represent?

This is the maximum frequency that will be shown on the frequency domain plot. This is equivalent to the Nyquist frequency of an FFT plot. Note that the sampling frequency used for any scan in Spectramag-6 is twice the Max frequency value set in the program.

What frequency range is used in a plot?

The range of the frequency plot is from DC to Max Frequency/2

How many samples can I acquire using the Spectramag-6 system?

The Spectramag-6 system can acquire a maximum of 700,000 data points per run, for example when the Single data acquisition mode is selected. When the Multiple data acquisition mode is selected and the user chooses to make N runs and acquire k samples per run, the Spectramag-6 program produces N files each with k samples.

What is the maximum sampling frequency that I can use for the Spectramag-6 system?

The maximum sampling frequency for the system is 10kHz. This is obtained by setting Max Frequency to 5kHz. However care should be taken in interpreting the obtained results as the –3dB point of the system is at 3.5kHz. Hence the bandwidth of the system is specified as from 0 – 3.5kHz.

Note: Depending on the host PC it is advisable to use a maximum sampling frequency of 10kS/s for Single acquisition and 5kS/s for Multiple acquisition.

What value should I set for the Number of Discrete Frequencies (NDF)?

Any value from 1–16 can be used but the best results are normally obtained when the Number of Discrete Frequencies (NDF) is set to 16. See Table 3 for number of data points required for different numbers of NDFs.

A.1.2. Coupling

When do I need to use the AC or DC coupling?

DC coupling is useful for coupling very slowly varying signals (quasi-DC or DC) of relatively small amplitudes. Note that AC signals will also be present when using DC coupling. A gain of 1 is generally suggested to avoid the saturation of the input amplifiers in the Spectramag-6 unit that have output ranges of $\pm 10\text{V}$. If however there is a need to measure a small AC signal that

is superimposed on/has a large DC offset, then AC coupling should be used to remove the DC component and acquire only the desired AC signal without saturating the input amplifiers in the Spectramag-6 unit.

What gain settings should I use?

The gain settings to be used depend on the magnitude of the signal to be acquired. To acquire quasi-DC/DC signals, DC coupling should be used with a gain of 1. If the input signal is a small AC and DC signal (say from a magnetometer) or purely an AC signal, then AC coupling should be used and a gain of >1 should be used to increase the overall signal-to noise ratio of the system (i.e. the ratio of the input signal relative to internal Spectramag-6's A/D converter noise).

A.1.3. Windowing

Which FFT window should I use?

Different FFT windows are chosen based on the types of signals being analysed and whether the point of interest is greater precision in determining the amplitudes or the frequencies of the spectral components in the frequency domain. Each window has its merits and demerits. **Table A.1** gives a summary of the different FFT windows available in the Spectramag-6 software and their uses. This should be used as a rough guide.

Table A.1: A summary of the FFT windows in Spectramag-6 and their uses

Type of Signal	Choice of Window	Frequency resolution	Amplitude Accuracy
Unknown content	Hann	Good	Fair
Narrowband random signal (e.g. vibration data)	Hann	Good	Fair
Sine wave or combination of sine waves	Hann	Good	Fair
Closely spaced sinusoids	Hamming	Good	Fair
Transient & synchronous sampling	Uniform	Best	Fair
Broadband random (white noise)	Uniform	Best	Poor
Random noise	Welch	Good	Fair
Random noise	Bartlett	Good	Fair

A.1.4. Data Acquisition

How do I save data after a run?

Data can be saved by the following actions:

- **File → Export → Graphics** This saves the data plots to a file.
- **File → Export → Data** This saves both the time and frequency domain data to a file.

Note: Data is automatically saved (as .sm6 files) when using the Multiple mode and additionally ASCII files can also be produced when this option is selected (see [Setting Acquisition Modes](#)). Data can also be saved manually as a .sm6 file using **File ->Save As**.

Is it possible to connect more than one Spectramag-6 units to my computer?

No. The Spectramag-6 software is designed to support only one Spectramag-6 unit connected to the computer via the USB port. Trying to run multiple Spectramag-6 programs or connecting more than one Spectramag-6 unit to the PC can cause the system to malfunction.

Where can I find further information on how to use the Spectramag-6 software?

A summary of how to use the Spectramag-6 software is given as a flowchart in **Figure A.2**. Available versions of the Spectramag-6 software can be downloaded from the Bartington Instruments website.

A.2: Spectramag-6 Data Acquisition Choices Flowchart

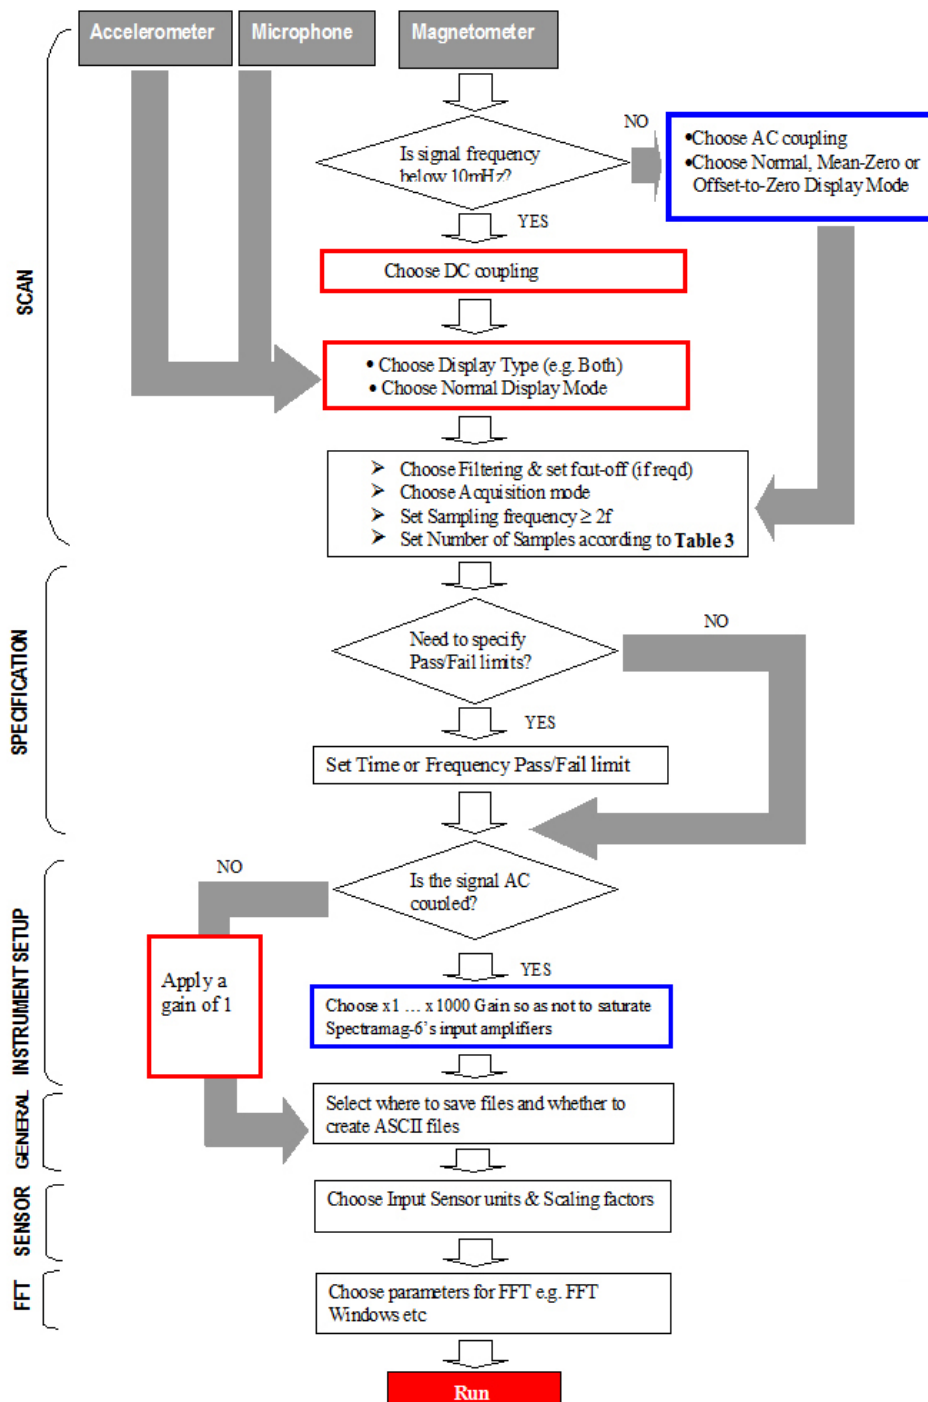


Figure A.2: Flowchart showing suitable choices for data acquisition using the Spectramag-6 software.

A.3. Spectramag-6 Do's and Don'ts

Do:

- Uninstall an older version of Spectramag-6 software before installing a new one.
- Switch OFF the Spectramag-6 unit, wait 10–15 seconds and restart the Spectramag-6 program if the USB cable is disconnected during a scan.
- Use Offset to Zero to remove DC bias/offset due to background fields in order to see a desired trend.
- Use the low-pass filter for removing power line signals and harmonics in order to see DC trends, for example while using DC coupling during site surveys. Note that the Nyquist criterion must be met, i.e. the sampling frequency used **MUST** be twice the minimum frequency content of the input signal.
- Close the Spectramag-6 program before disconnecting the USB.
- Ensure that there is enough storage space on the hard disk before using the Multiple data acquisition mode.

Don't:

- Have other programs running on the PC while running the Spectramag-6 program, especially when acquiring data from multiple inputs.
- Apply gain while using DC coupling (for magnetometer inputs).
- Use **Mean Zero** if you are interested in slow trends e.g. while using DC coupling.
- Under-sample your signal during data acquisition. The Moving Average low-pass filter is after the A/D converter, hence it is not suitable as an anti-aliasing filter.
- Use low-pass filtering if you are interested in plotting AC signal outside the passband of the low-pass filter.
- Allow multiple Spectramag-6 program windows to be open at one time. This could slow down and also affect the performance of the program.
- Tick the Display Specific Curve Box when the Time Domain or Frequency Domain Specification is used unless a suitable Excursion limit has been set.

When Time Domain or Frequency Domain Specification is used (and the Display Specific Curves option is selected), the auto-scale is disabled and the Maximum Excursion specified by the user is used as the plot range. If the range specified is much larger than the actual signal then only straight lines will be seen. In that case the zoom option should be used by holding down the left mouse and dragging a box around an

area of interest to zoom in. Alternatively a suitable excursion limit should be specified or the Display Specific Curve box should not be ticked.

- Install the Spectramag-6 program on very low spec computers as this will affect the performance of the program and can also lead to unpredictable results. See [Hardware](#) for the minimum computer specification.
- Acquire data using the Spectramag-6 system when the Spectramag-6 unit doesn't have adequate charge.
- Use **Data → Copy** when large data has been acquired. Large data should be exported to a file by **File → Export → Data**.
- Try to connect more than one Spectramag-6 units to one computer. The Spectramag-6 system is currently designed so that only one unit can be connected to each computer.

Appendix B

B.1. Spectral Analysis using Fourier Transforms

B.1.1. Introduction

Most real life sensors and transducers provide signals, usually as a function of time. Such signals can be represented visually in equipment such as oscilloscopes, chart recorders etc. By representing signals as a function of time it is easy to derive information such as the amplitude, period and frequency (for a simple sinusoid). However most real life signals are complex signals consisting of a mixture of transients, sinusoids, noise etc. When complex signals are represented as a function of time, it is still possible to derive information about the amplitude and duration of the complex signal. However it is most often impossible to determine the frequency and there is no information concerning the amplitude, frequency and phase of the constituent signals. Such information is vital in many engineering disciplines and is essential in determining how systems such as amplifiers, filters etc will respond to a particular signal. It is therefore necessary to represent complex signals not only as a function of time but equally as a function of frequency. This is achieved by Fourier analysis.

B.1.2. Fourier Series and Transforms

One of the key foundations for frequency analysis was laid by Jean Baptiste Joseph Fourier in 1822 when he stated that any periodic motion can be written as a superposition of sinusoidal and cosinusoidal vibrations. This forms the basis of what is now known as Fourier Series (used for periodic signals); which was extended to Fourier Transform (to deal also with aperiodic signals); then to Discrete Fourier Transform (to deal with sampled/digital signals); and finally to Fast Fourier Transform, which is a faster version of the Discrete Fourier Transform.

B.1.3. Processing digital signals

The advent of the digital computer led to the realisation of and the continual drive for processing signals digitally – a field now known as Digital Signal Processing (DSP). Most real life transducers are analogue in nature, hence the first step to digital signal processing is the analogue-to-digital (A/D) signal conversion. This process allows a time-varying analogue signal to be represented digitally. During the analogue to digital conversion, a signal is first sampled and the values obtained are then represented digitally. The rule for correctly sampling a signal was set by the Nyquist theory (according to the work of Harry Nyquist) which stated that to define a signal correctly, it is necessary to take at least two samples during each cycle of the signal. If the signal consists of a mixture of frequencies then the sampling rate chosen should be at least twice that of the highest frequency component. Sampling a signal at twice its frequency ensures that a signal can be reconstructed (after processing) and that its frequency can be accurately measured. However the Nyquist rate does not guarantee accurate representation of the signal's shape or amplitude. Oversampling the signal at ten times the Nyquist rate is mostly given as a rule of thumb.

On the other hand, if a signal is undersampled, i.e. sampled at less than the Nyquist rate, all the signals over half the sampling frequency (the Nyquist frequency) are folded back or mirrored back into the pass region according to **Equation B1**. This is as shown in **Figure B.1**. Once a signal is aliased, it is practically difficult to recover the original signal.

$$f_{alias} = c * f_{samp} - f_{signal} \quad (B1)$$

where:

- f_{alias} is the alias frequency
- f_{samp} is the sampling frequency
- f_{signal} is the original signal frequency
- c is an integer multiple of the sampling frequency such that it is closest to f_{signal}

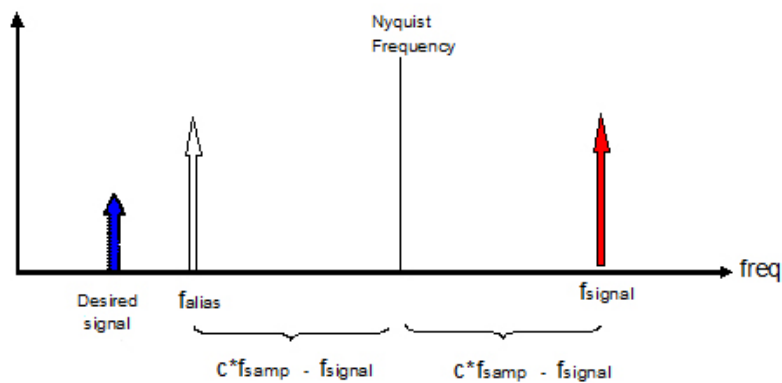


Figure B.1: Aliasing due to undersampling a signal.

B.1.4. FFT windows

FFT assumes the periodicity of any input waveform and the existence of this waveform from plus infinity to minus infinity. In reality, waveforms often being processed exist for a fixed duration and FFT therefore assumes that a waveform is repeated for all time. If the input waveform consists of **non-integral cycles**, there will be discontinuities when it is repeated. Hence FFT sees these 'bogus' discontinuities that weren't there in the original signal. The Fourier Transform of a signal with these discontinuities produces (along with the spectral components) spurious signals spread across all the FFT bins. This causes spectral leakage where power leaks from each spectral component to all other bins. The leakage from strong spectral components often completely swamps weaker components, making them hard to detect or resolve in frequency. The use of FFT windows is therefore necessary to reduce the effect of spectral leakage that occurs due to end-to-end mismatch **because it is not always possible to guarantee that the data being used in an FFT represents an integral cycle** of the acquired signal. The following are typical scenarios:

1. Assume that one desires to perform a 1024-point FFT of a signal. In this case, one can acquire 1024 data points of the signal. If the signal is a single periodic sinusoid, the sampling rate can be chosen so that complete cycles of the signal can be acquired

using the 1024 data points. In reality, most signals that are analysed are complex signals consisting of multiple frequencies hence such approach is not useful.

2. Using the same example in (i), assuming that a longer dataset of 65536 points was acquired and one desires a 2048-point FFT; the 65536 data points have to be divided into 32 data segments each of which will be FFTed separately. Again, it is difficult to ensure that each 2048 block of data represents a complete cycle of the input signal.
3. In some cases (such as noise analysis) it is equally hard to determine the exact period of a signal in order to acquire data corresponding to complete cycles of the waveform.

The above points make it useful to window each data before they are FFTed. Different FFT windows lead to different amplitude accuracies and frequency resolution, hence an appropriate window should be selected depending on the signal being processed. For example the Hamming window is good for analysing closely spaced frequencies. It gives the best frequency resolution but not the optimal amplitude accuracy. A Hann window on the other hand is good for analysing narrowband random signals, combination of sinusoids or signals of unknown content. It gives slightly better amplitude accuracy but poorer frequency resolution compared to the Hamming window.

Hence the choice of a window depends on the signal being processed and whether the point of interest is signal detection or frequency resolution. Another point to note is that a signal of finite duration (as mentioned previously) is seen by FFT as a signal of infinite duration to which a Rectangular window was applied. As such, even when no generic window function has been applied to a signal, due to the finite existence of the signal, FFT assumes that the Uniform (None) window has been used. The Uniform (Rectangular or None) window therefore represents a case when no window function has been applied.

B.2.Sampling and Logging Time Estimates

Table B.2 gives estimates of the logging time that can be achieved with different sampling rates using the Spectramag-6 software.

Table B.2: estimates of the logging time that can be achieved with different sampling rates using the Spectramag-6 software.

Sampling rates	Data points per run	Logging/Acquisition time			
		1 Run (sec)	50 Runs (hrs)	100 Runs (hrs)	150 Runs (hrs)
10kS/s	700,000	70	0.97	1.94	2.92
5kS/s	700,000	140	1.94	3.88	5.83
2.5kS/s	700,000	280	3.88	7.78	11.67
1kS/s	700,000	700	9.72	19.4	29.20 (1.21 days)
500S/s	700,000	1400	19.4	38.88 (1.62 days)	58.30 (2.43 days)
200S/s	700,000	3500	48.6 (2 days)	97 (4 days)	145.8 (6 days)
100S/s	700,000	7000	97.20 (4 days)	194 (8 days)	291.66 (12 days)

Notes



Bartington® Instruments

T: +44 (0)1993 706565
F: +44 (0)1993 774813
E: sales@bartington.com

Bartington Instruments Limited
5 Thorney Leys Business Park,
Witney, Oxford, OX28 4GE, England.

www.bartington.com

The copyright of this document is the property of Bartington Instruments Ltd.
Bartington® is a registered trade mark of Bartington Instruments Limited in the following countries:
United Kingdom, Australia, Brazil, Canada, China, European Union, India, Japan, Norway and the
United States of America.