

DESCRIPTION

The *SENIS* 3-Axis AC Magnetic Transducer 3DACMT-1 is a compact instrument to measure all 3 components of alternating magnetic fields with very high resolution in a small volume.

It incorporates three groups of mutually orthogonal coils, analog integrators and amplifiers within a small cube and generates 3 high level output signals that are immune to electromagnetic disturbances. The sensing cube is completely non magnetic and therefore does not disturb the external field.

The *SENIS* 3DACMT-1 Transducer is ideally suited to measure and map AC magnetic fields in noisy environments with field resolution better than $1.5\mu\text{T}$.

KEY FEATURES

- Frequency range from 10kHz to 200kHz
- Magnetic field resolution better than $1.5\mu\text{T}_{\text{rms}}$
- Small probe volume of about 3.6 cm^3
- Non-invasive: The probe does not modify the measured magnetic field
- Highly linear response
- High transduction accuracy of $\pm 1\%$
- High phase accuracy: $< 3^\circ$ at 85kHz
- Excellent angular accuracy $< \pm 1^\circ$
- Negligible cross-talk
- Common center of coils for all three axis
- Insensitive to electrical fields or capacitive coupling
- Analog output

PRELIMINARY TECHNICAL SPECIFICATIONS

Geometrical	Value
Size of sensing cube, A	15.3mm x 15.3mm x 15.3mm
Probe length (sensing cube with holder), L1	240mm
Cable length, L	3m \pm 10cm
Size electronic box (BxCxD)	150mm x 38mm x 95 mm
Orthogonality of different sensing directions	$< 1^\circ$ in all 3 Cartesian directions
Electrical	
Full measurement range	$\pm 10\text{mT}$
Output Signal	Bipolar, single—ended, amplitude from 0V to $\pm 5\text{V}$
Sensitivity	500mV/mT
Magnetic resolution	Better than $1.5\mu\text{T}_{\text{rms}}$ for all three axis
Magnetic nonlinearity	$< 1\%$ for $f < 100\text{kHz}$
Measurement bandwidth	10kHz - 200kHz
Phase shift	Better than 3° at 85kHz
Minimum Load Impedance	$10\text{k}\Omega$
Output resistance	$< 60\Omega$
Spurious in measurement range	$< 100\mu\text{V}_{\text{peak}}$ ($< 200\text{nT RTI}$)
Current consumption	$\pm 45\text{mA}$ @ $\pm 12\text{V}$

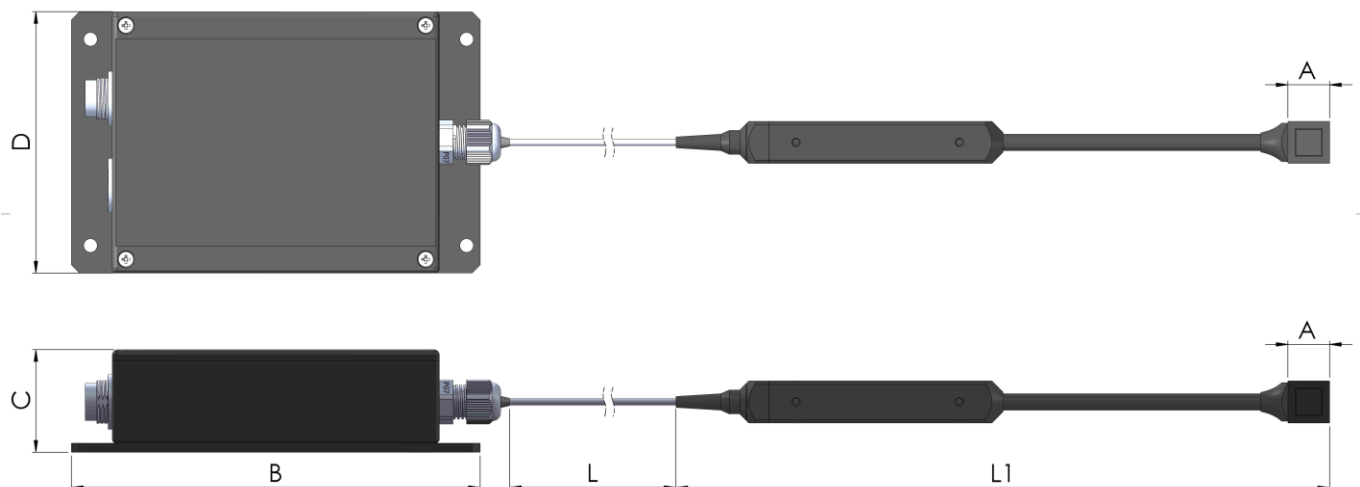


Figure 1. Geometry of the AC Transducer and Probe



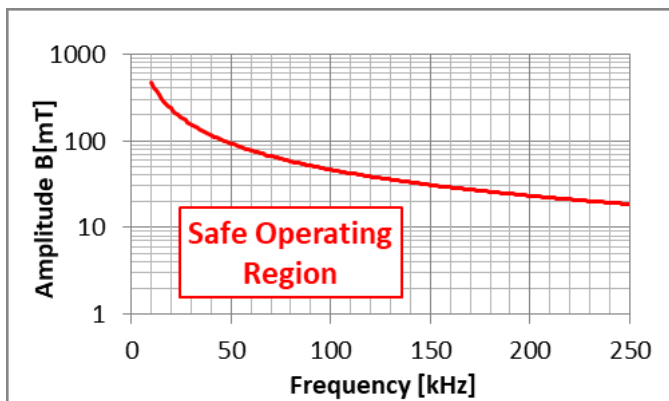


Figure 2a: Safe Operating Region

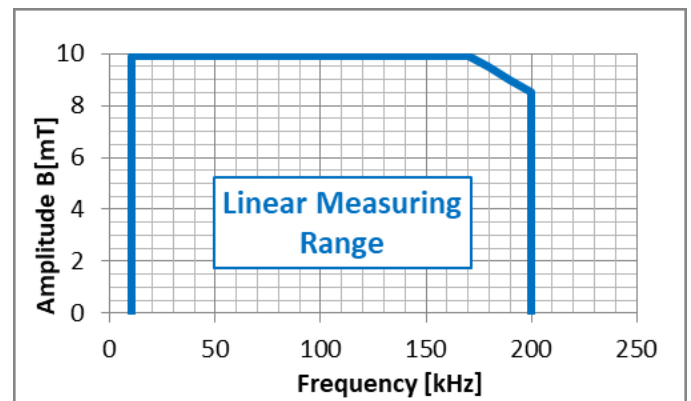


Figure 2b: Linear Measuring Range

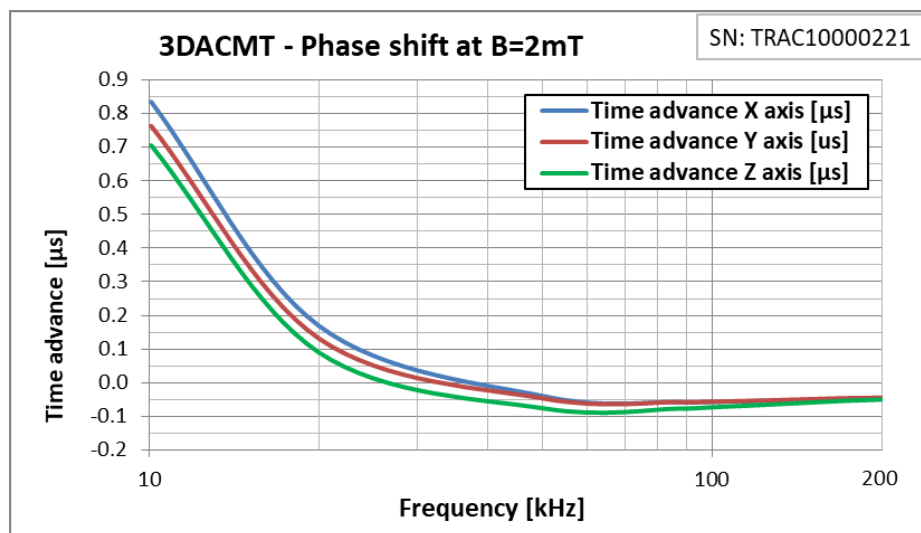


Figure 3: Time advance for all three axes.

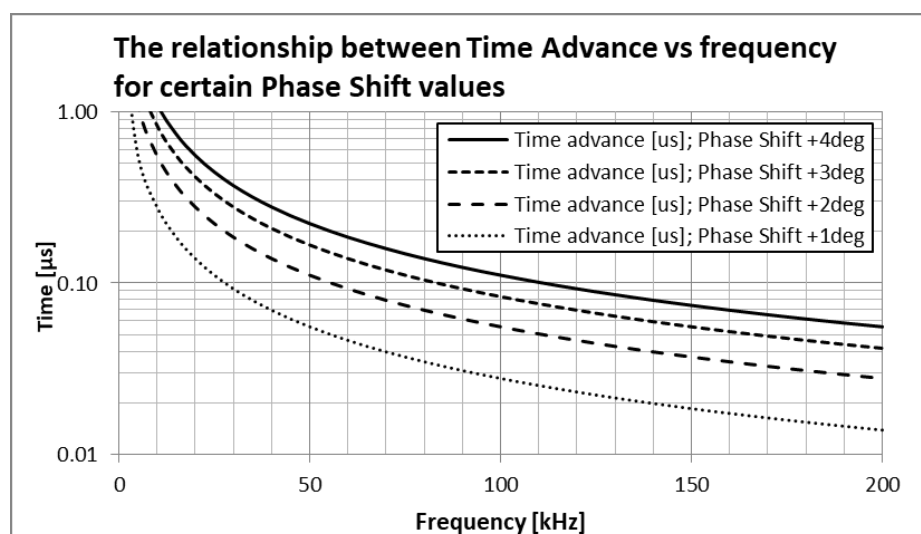


Figure 4: Relationship between Time Advance vs. frequency.



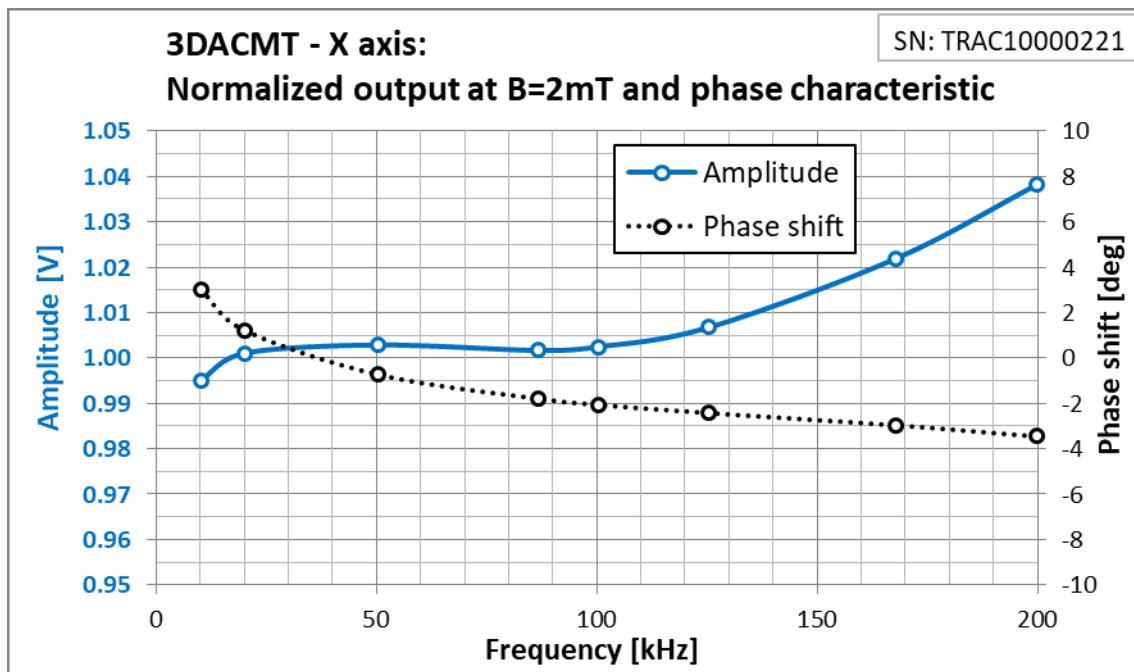


Figure 5: X axis - Normalized Output and Phase Shift.

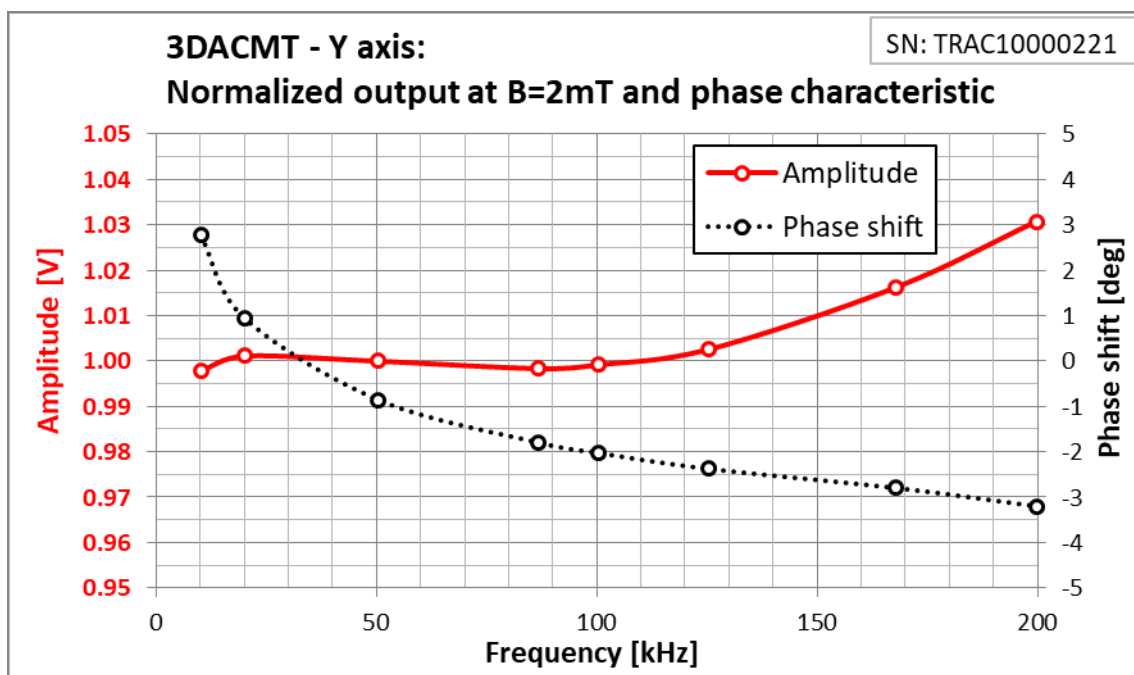


Figure 6: Y axis - Normalized Output and Phase Shift.

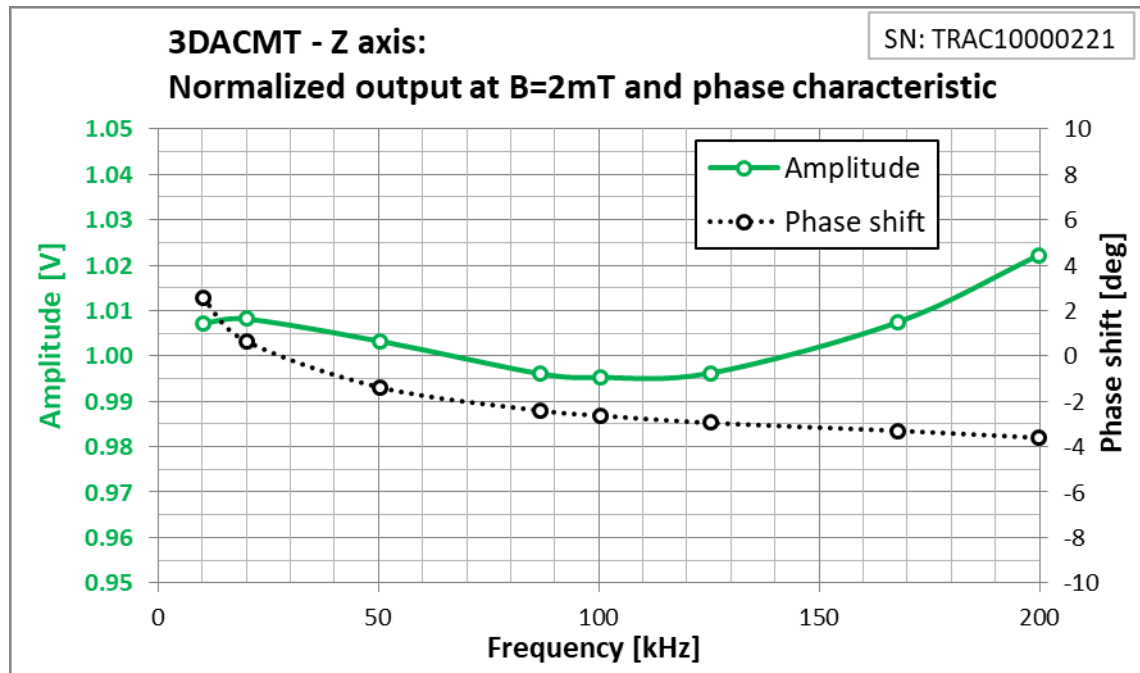


Figure 7: Z axis - Normalized Output and Phase Shift.

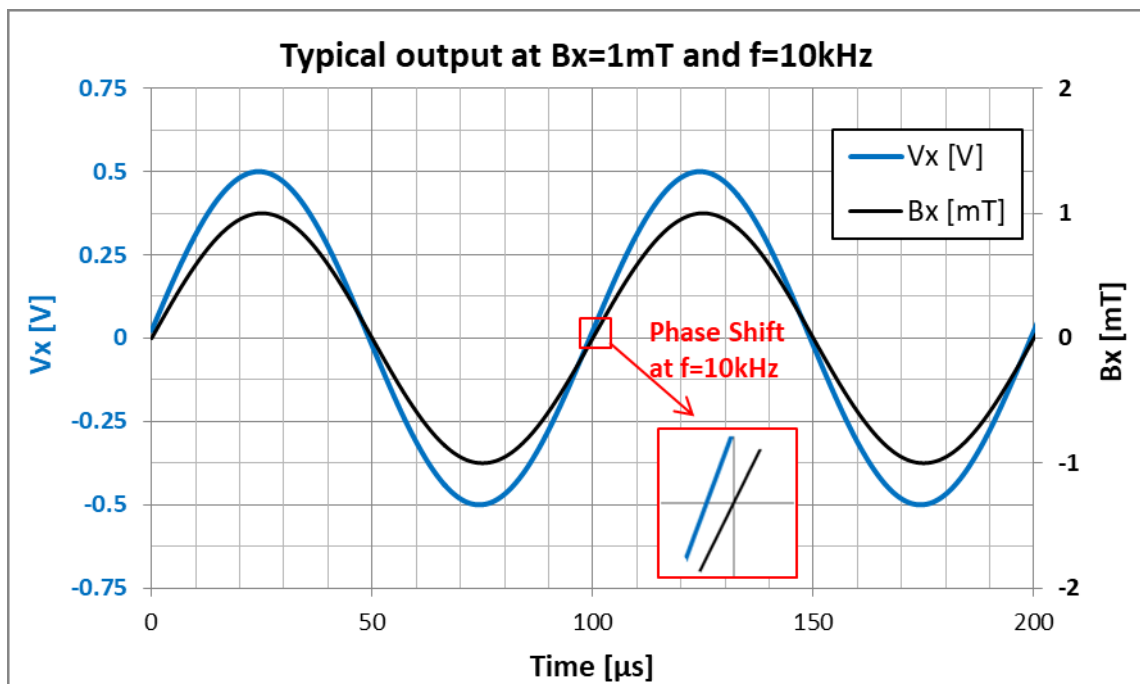


Figure 8: Typical output at B=1mT and f=10kHz

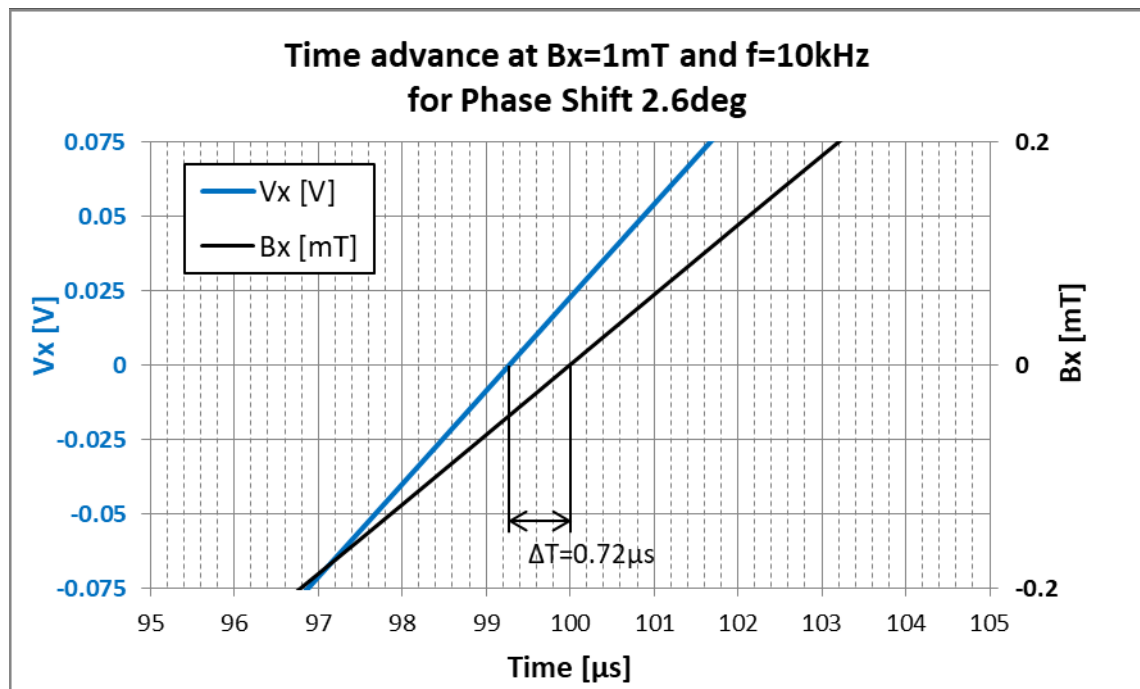


Figure 9: Time advance at zero-crossing for $B_x=1\text{mT}$ and $f=10\text{kHz}$ and Phase Shift 2.6°



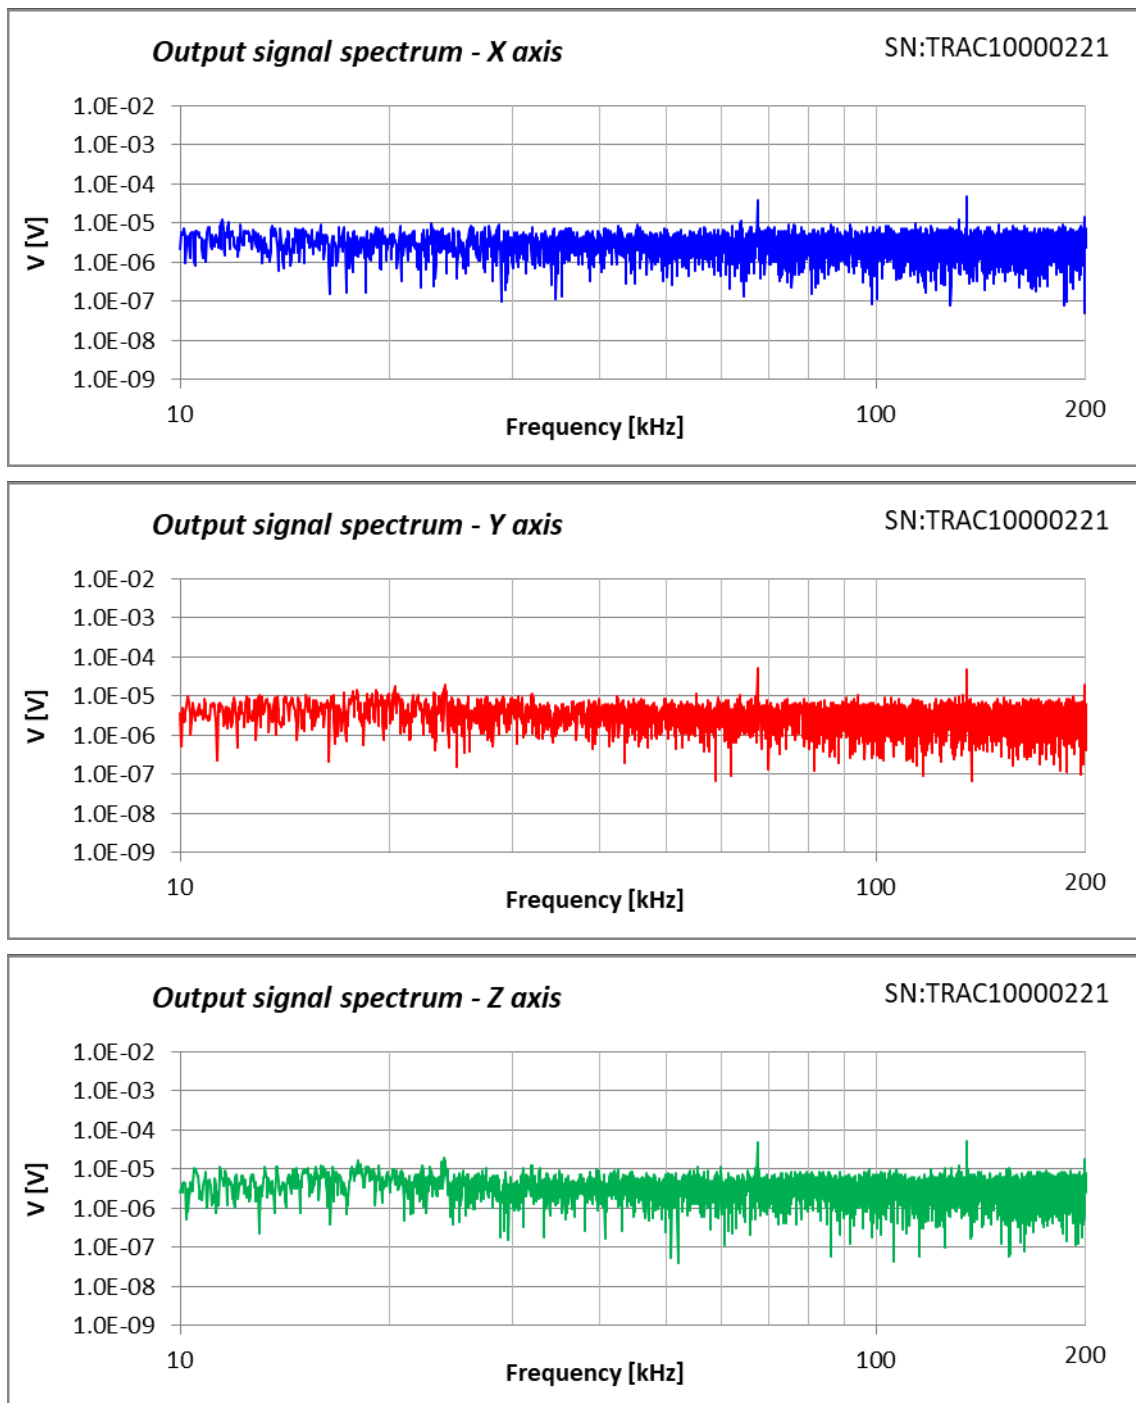


Figure 10: Spectrum of the output signals at $B=0T$.



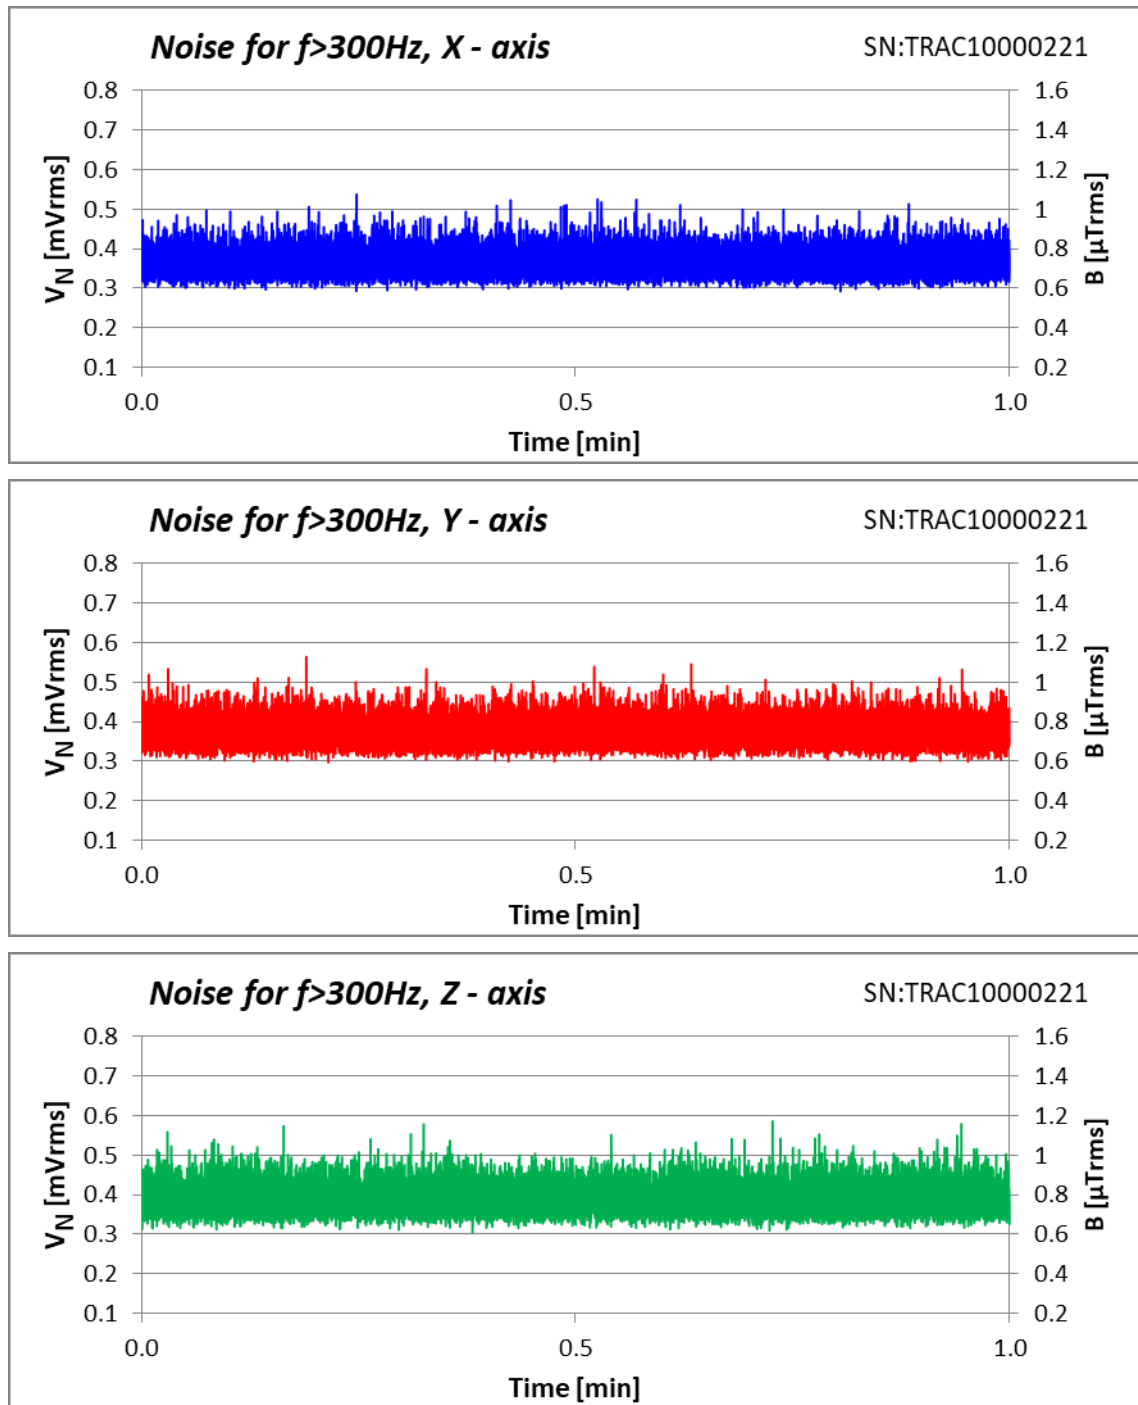


Figure 11: Typical Noise for $f > 300\text{Hz}$, rms Value.



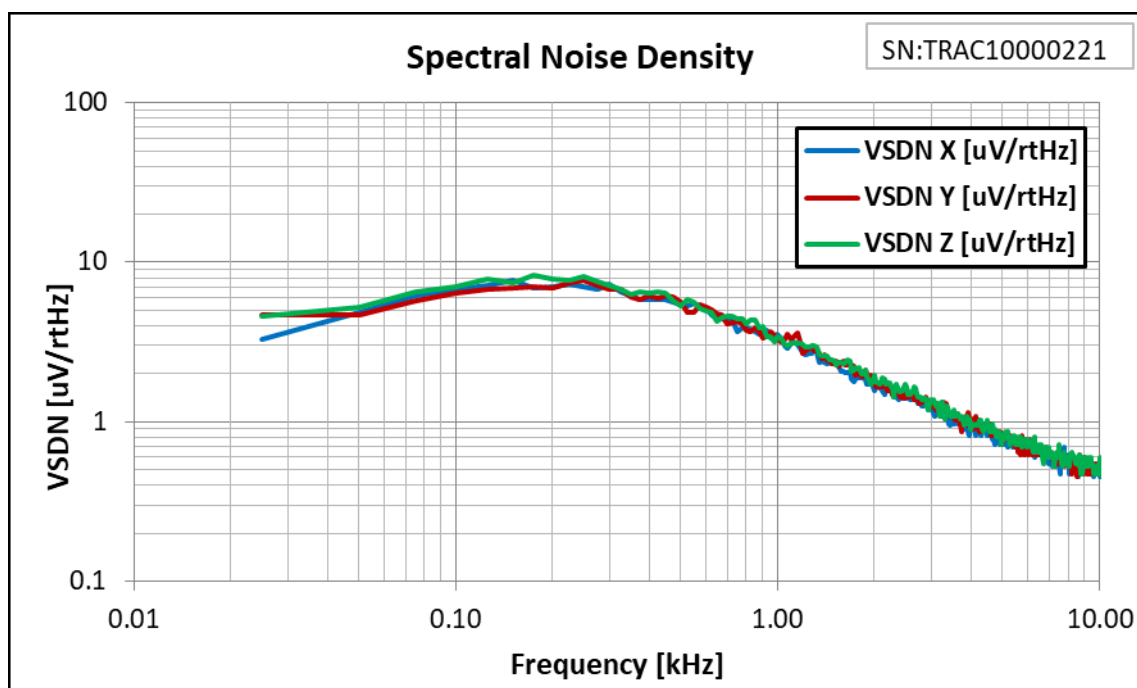


Figure 12: Spectral Noise Density.

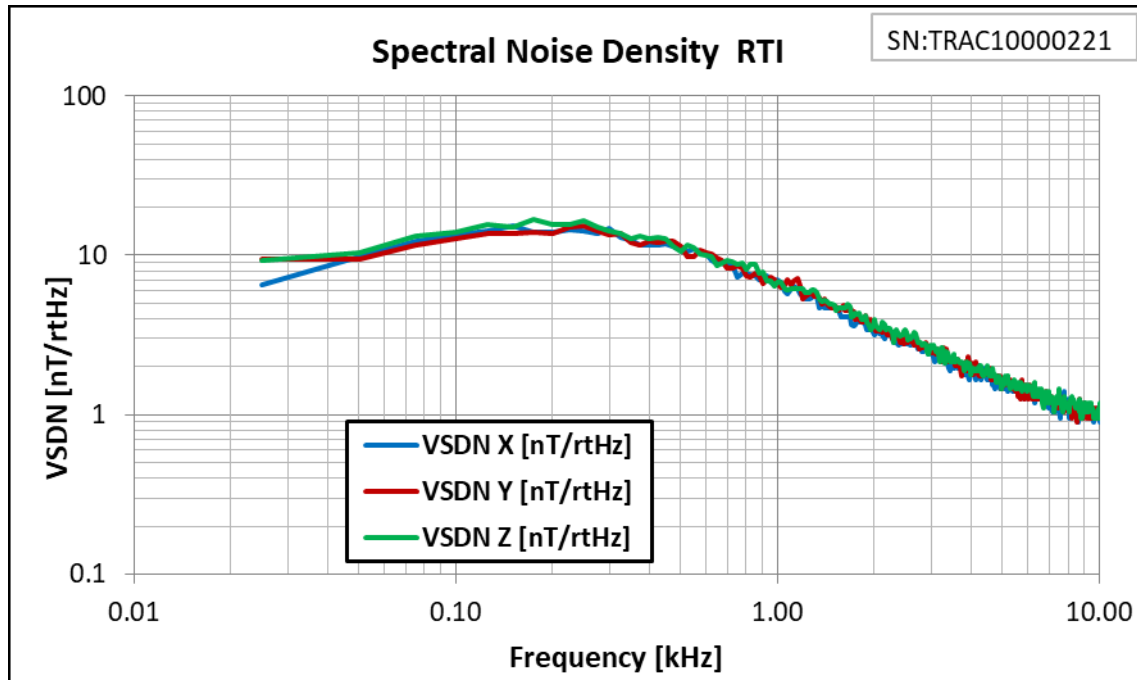


Figure 13: Spectral Noise Density RTI (Referred To Input).



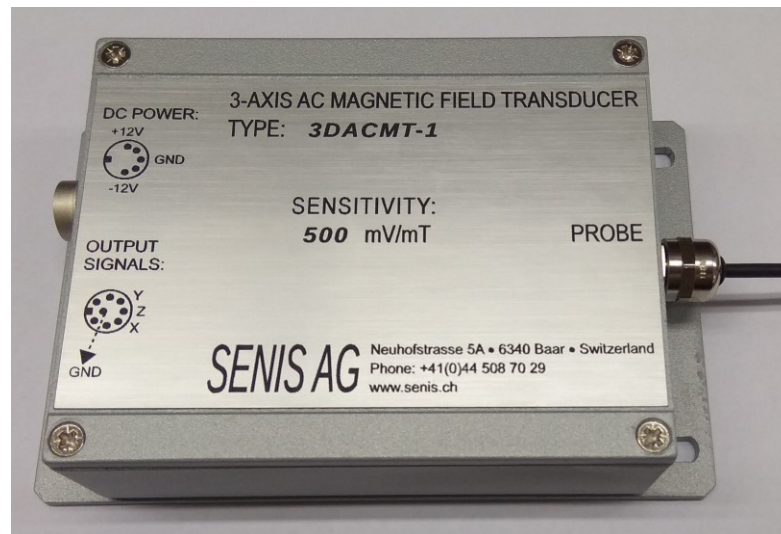


Figure 14: Photo of 3D AC Magnetic Field Transducer.



Figure 15: Probe photo.



Pin No.	Output signal
1	Not used
2	Z axis
3	Not used
4	X axis
5	Y axis
6	Not used
7	Not used
8	GND (Common)

Figure 16: Output signal connector KVF 81 (matching with cable SV81 connector - pin out, front view)



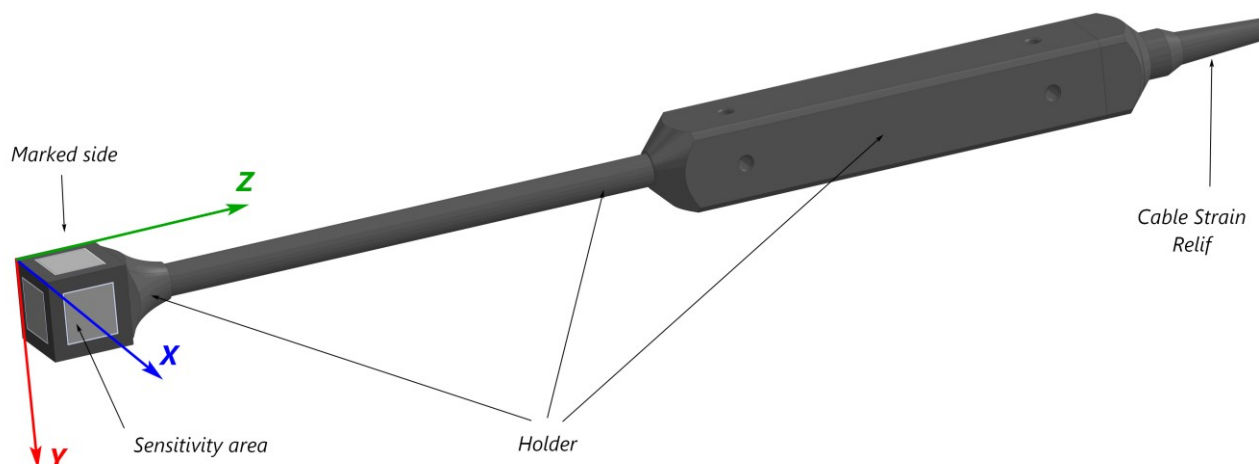


Figure 17: Probe – drawing.

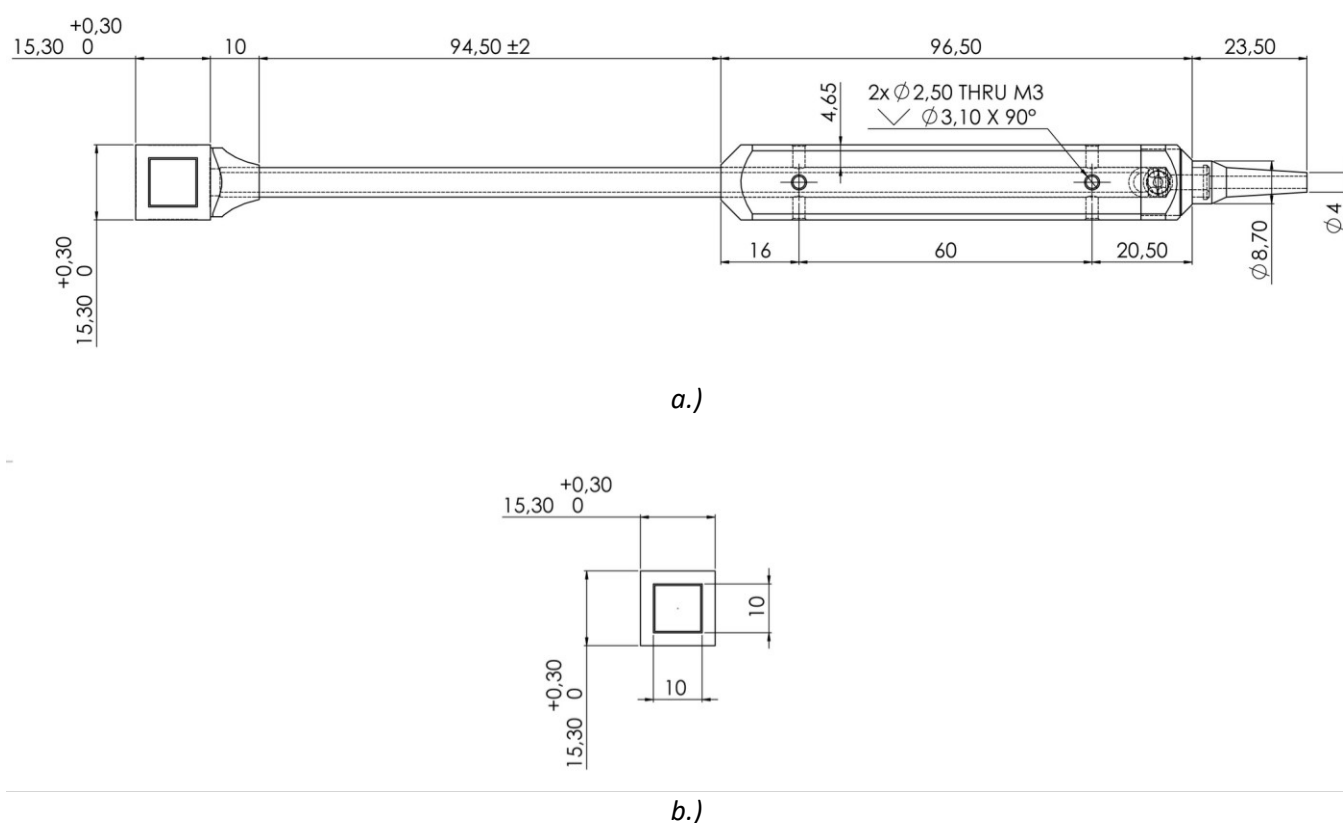


Figure 18: Probe – dimensions (all dimensions are in mm):

a.) – Side View;
b.) – Front View.

Appendix A

Relations between Power Supply AC lines, Common and +/- voltage rails

Connection between Power Supply S12-5 and 3DACMT-1 is given of Figure a1.

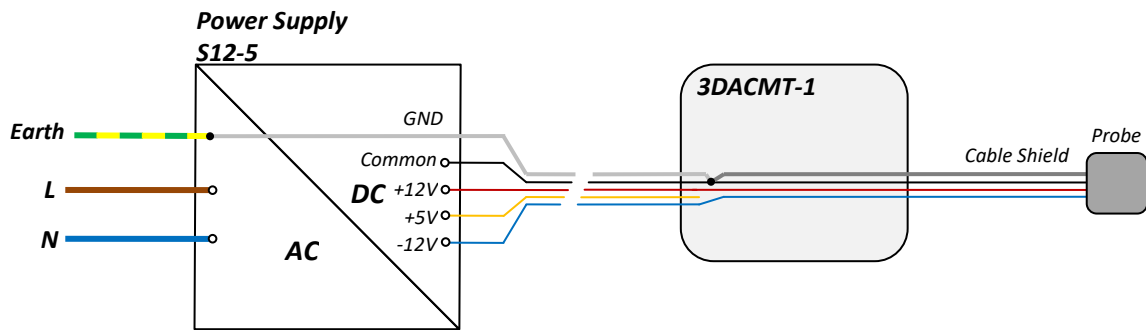


Figure a1.

On Figure a2 is given shield connection of Power Supply S12-5.

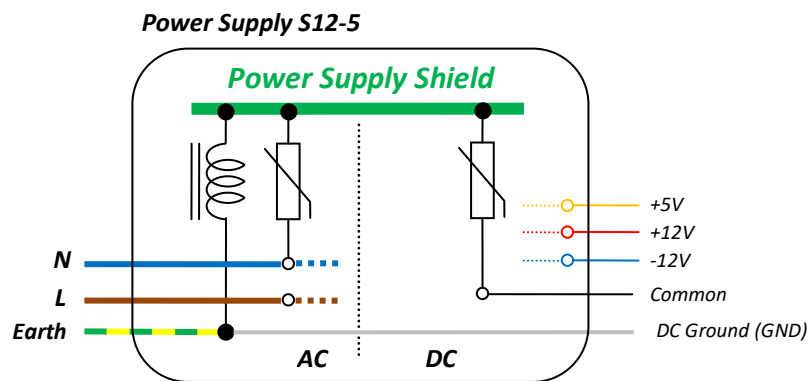


Figure a2.

Appendix B

3DACMT-1 calibration Set-up

Calibration Set-up is given of Figure b1.

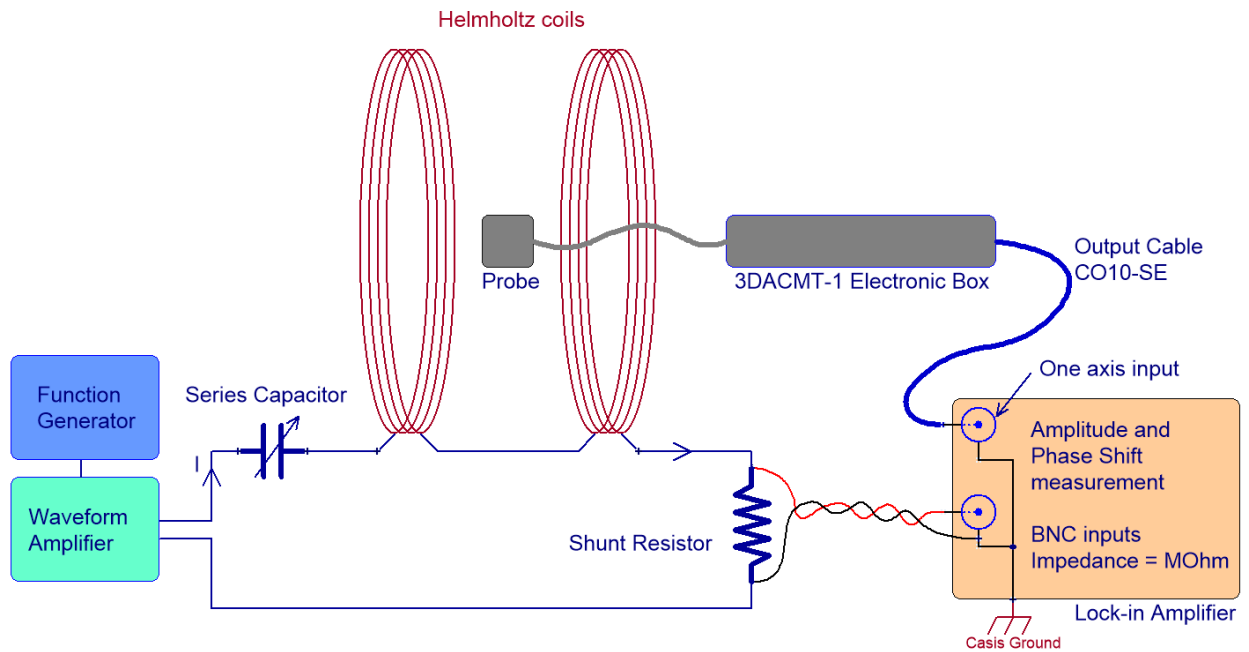


Figure b1.

